
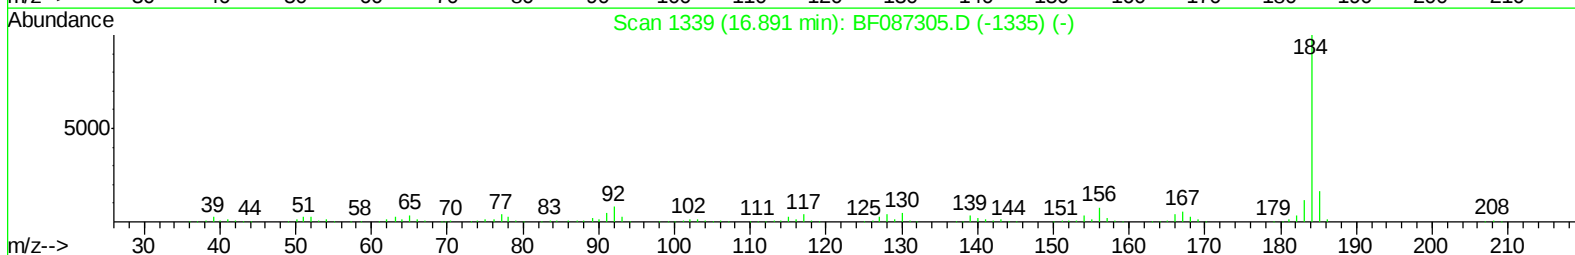
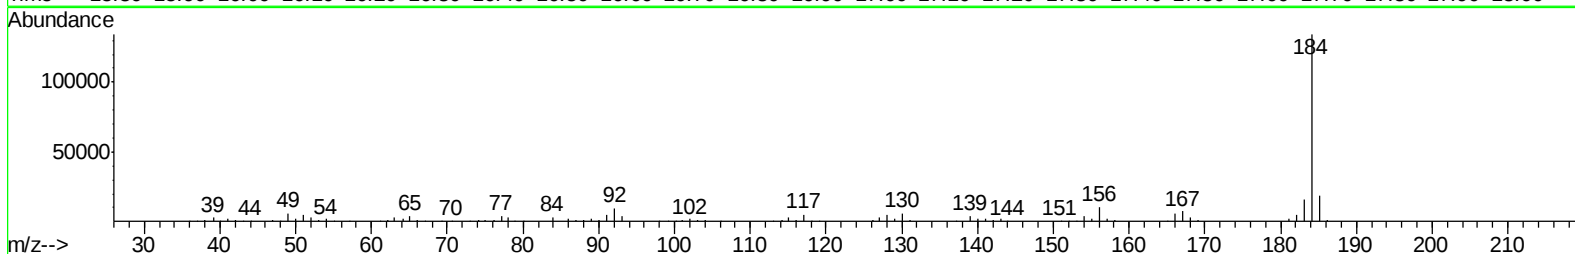


Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF052416\  
Data File : BF087344.D  
Acq On : 24 May 2016 18:38  
Operator : UM/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 25 06:49:45 2016  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF052316.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed May 25 00:58:25 2016  
Response via : Initial Calibration

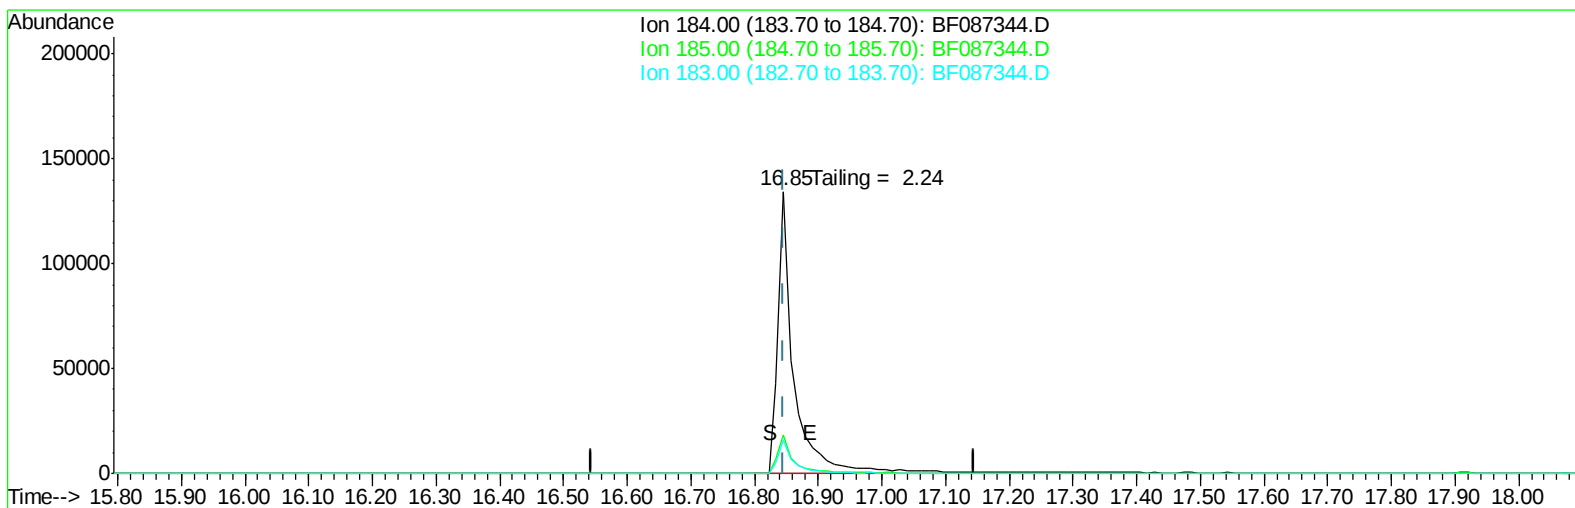

TIC: BF087344.D

(76) Benzidine




16.846min (-0.000) 0.00ng

response 230161

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 17.00 | 13.88 |
| 183.00 | 12.20 | 11.76 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF052416\  
Data File : BF087344.D  
Acq On : 24 May 2016 18:38  
Operator : UM/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 25 06:49:45 2016  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF052316.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed May 25 00:58:25 2016  
Response via : Initial Calibration

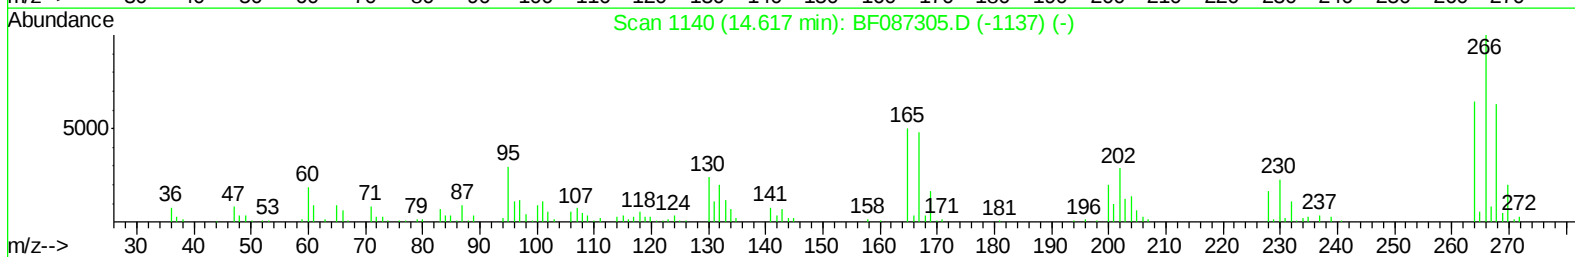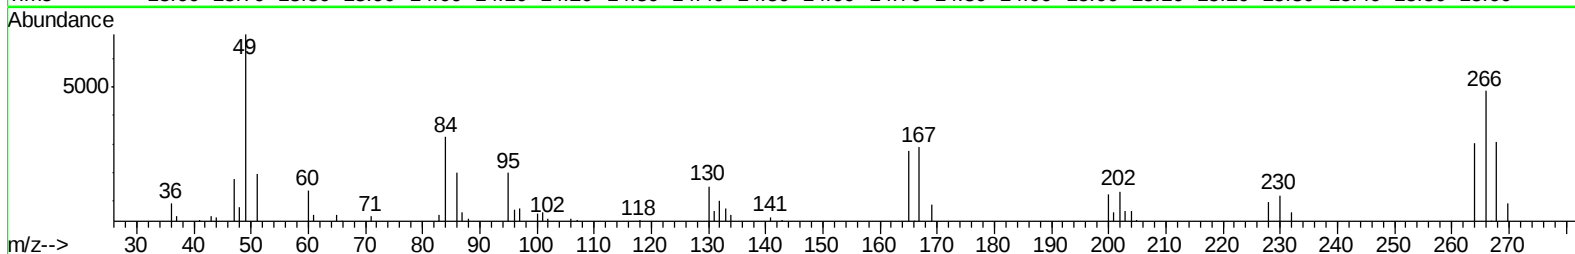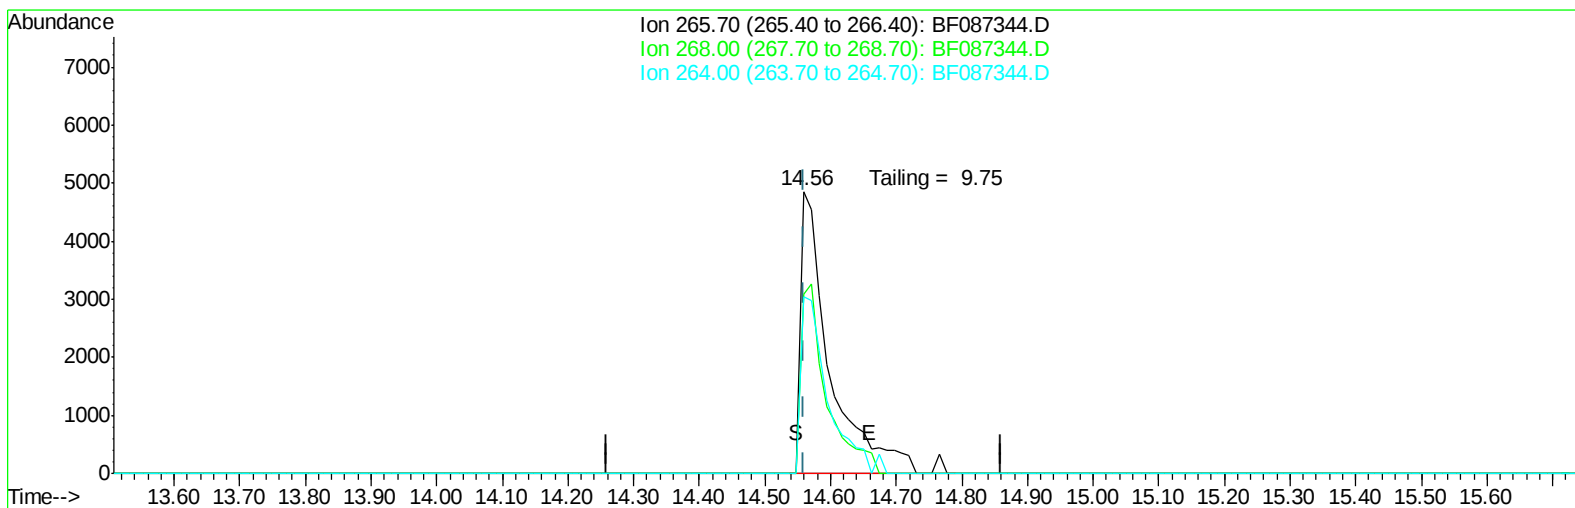

TIC: BF087344.D

(69) Pentachlorophenol (C)

14.560min (-0.000) 0.00ng

response 14733

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 64.40 | 63.49 |
| 264.00 | 66.10 | 62.79 |
| 0.00   | 0.00  | 0.00  |