

Data Path : Z:\HPCHEM1\BNA F\DATA\BF052416\
 Data File : BF087364.D
 Acq On : 25 May 2016 5:51
 Operator : UM/SJ
 Sample : H3191-13
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CHS-STA-1685(0-4)

Quant Time: May 25 06:49:15 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF052316.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 25 00:58:25 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	114749	20.00	ng	0.00
21) Naphthalene-d8	9.59	136	459482	20.00	ng	-0.01
38) Acenaphthene-d10	12.41	164	221162	20.00	ng	-0.01
63) Phenanthrene-d10	14.82	188	453187	20.00	ng	0.00
75) Chrysene-d12	18.50	240	380664	20.00	ng	-0.01
86) Perylene-d12	20.17	264	272743	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.48	112	919392	140.79	ng	0.02
7) Phenol-d6	7.10	99	1136483	128.79	ng	-0.01
23) Nitrobenzene-d5	8.47	82	858761	94.19	ng	-0.02
41) 2,4,6-Tribromophenol	13.71	330	350039	164.70	ng	-0.01
44) 2-Fluorobiphenyl	11.37	172	1525826	97.26	ng	-0.01
78) Terphenyl-d14	17.17	244	1598544	89.28	ng	-0.01
Target Compounds						
31) Naphthalene	9.62	128	134604	5.85	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF052416\
Data File : BF087364.D
Acq On : 25 May 2016 5:51
Operator : UM/SJ
Sample : H3191-13
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CHS-STA-1685(0-4)

Quant Time: May 25 06:49:15 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 25 00:58:25 2016
Response via : Initial Calibration

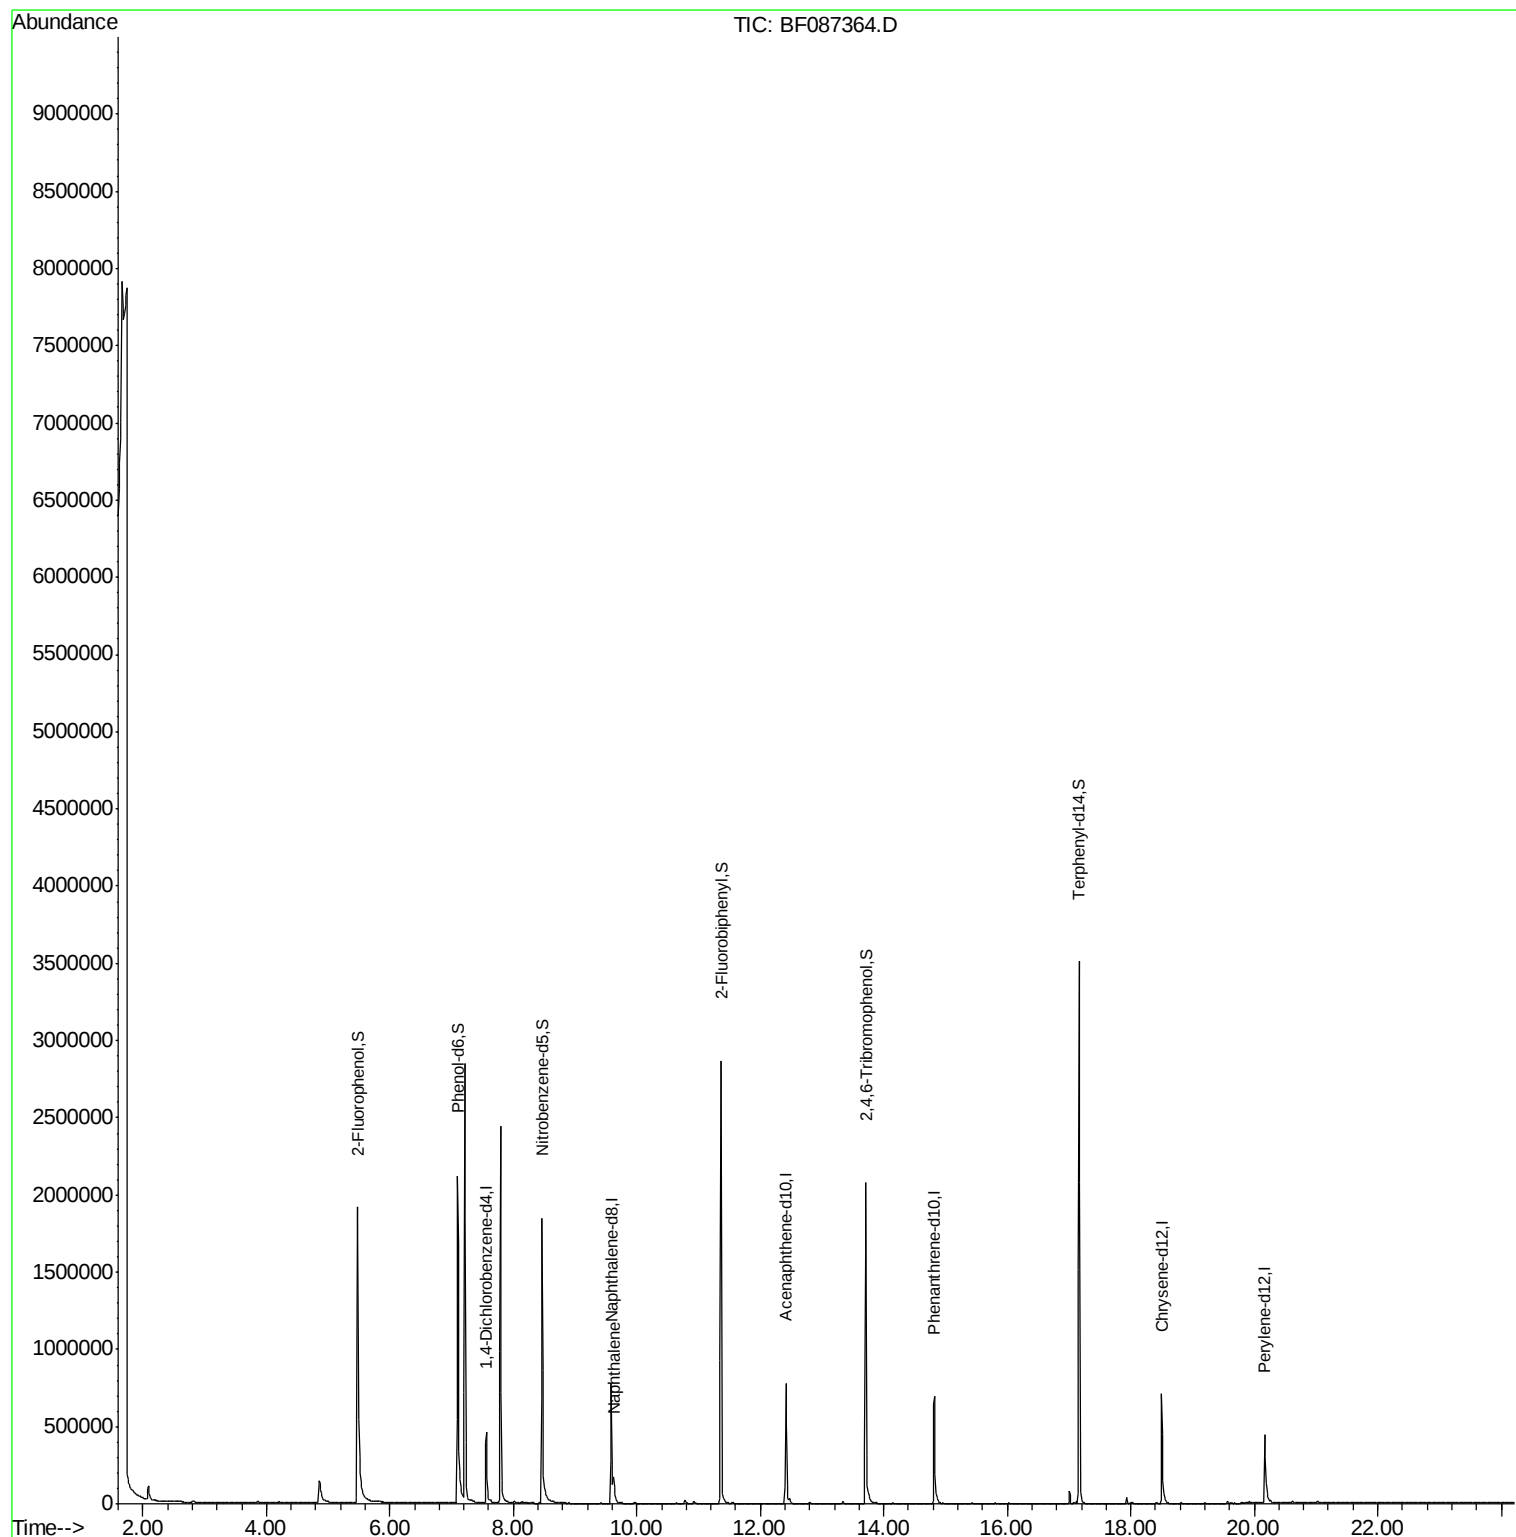

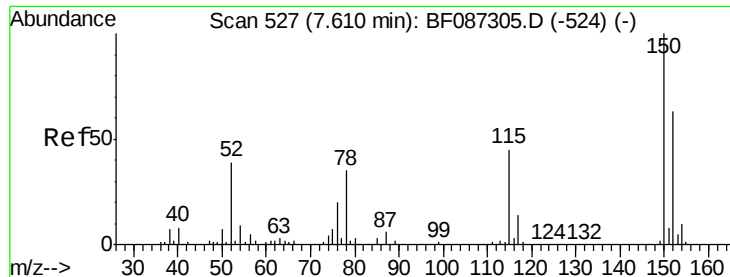

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 7.56 min Scan# 523

Delta R.T. 0.00 min

Lab File: BF087364.D

Acq: 25 May 2016 5:51

Instrument :

BNA_F

ClientSampleId :

CHS-STA-1685(0-4)


Tot Ion:152 Resp: 114749

Ion Ratio Lower Upper

152 100

150 155.6 125.8 188.6




115 62.2 51.5 77.3

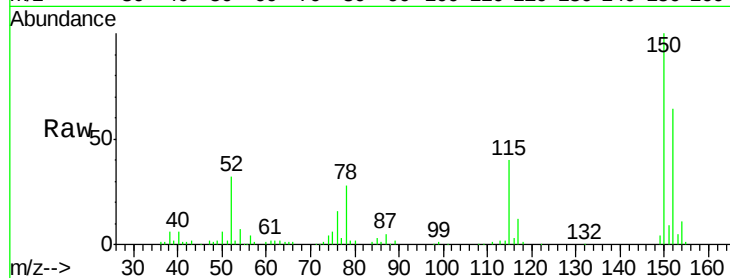

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

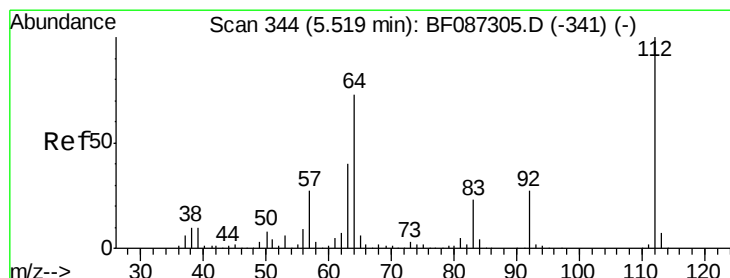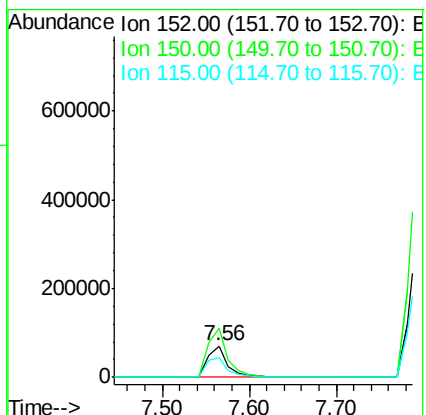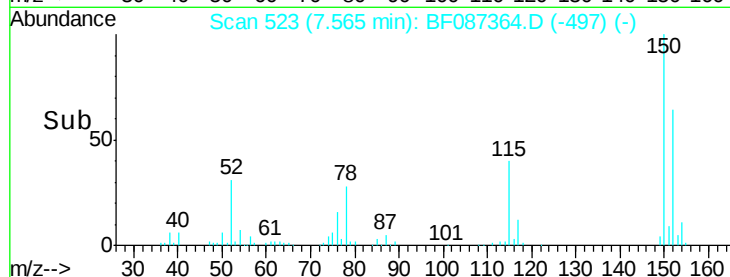

#5

2-Fluorophenol

Concen: 140.79 ng

RT: 5.48 min Scan# 341

Delta R.T. 0.02 min

Lab File: BF087364.D

Acq: 25 May 2016 5:51


Tgt Ion:112 Resp: 919392

Ion Ratio Lower Upper

112 100

64 65.2 52.1 78.1



63 35.9 25.7 38.5

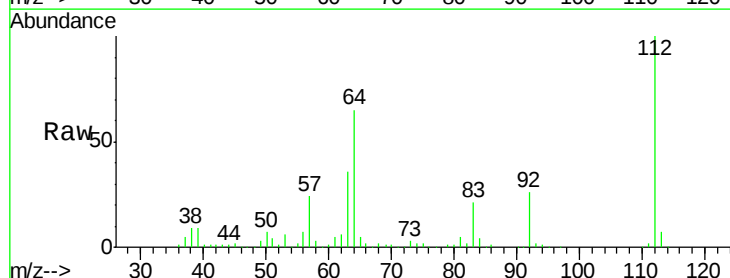


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

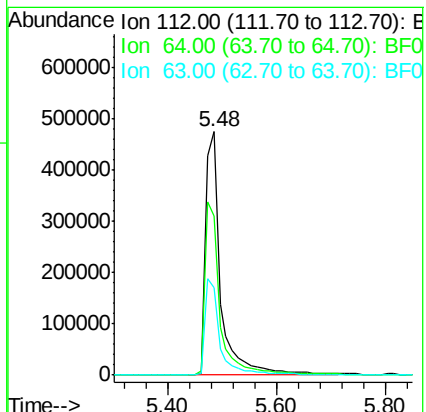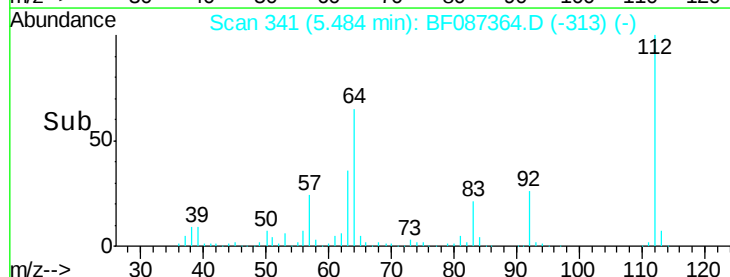

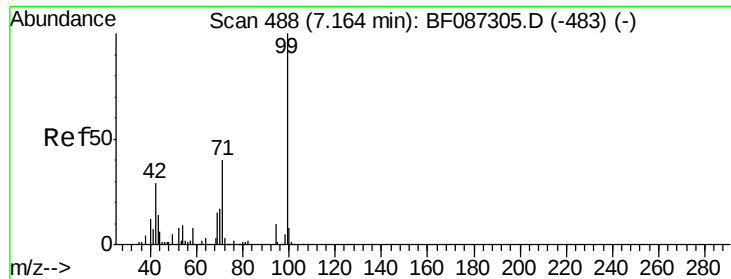

#7

Phenol-d6

Concen: 128.79 ng

RT: 7.10 min Scan# 482

Delta R.T. -0.01 min

Lab File: BF087364.D

Acq: 25 May 2016 5:51

Instrument :

BNA_F

ClientSampleId :

CHS-STA-1685(0-4)





Tot Ion: 99 Resp: 1136483

Ion Ratio Lower Upper

99 100

42 31.5 13.6 20.4#

71 41.5 24.6 36.8#

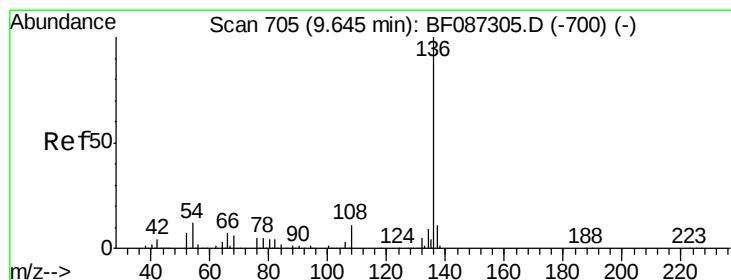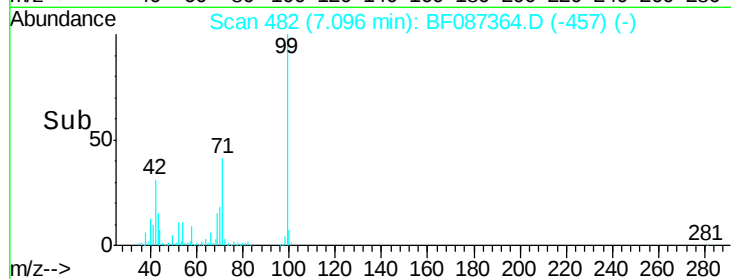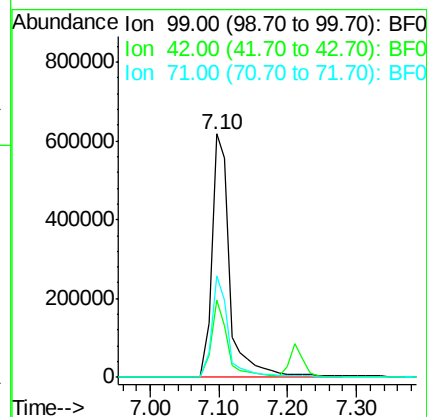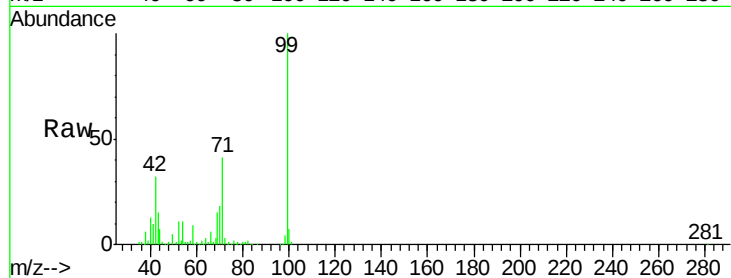

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 9.59 min Scan# 700

Delta R.T. -0.01 min

Lab File: BF087364.D

Acq: 25 May 2016 5:51

Tgt Ion: 136 Resp: 459482




Ion Ratio Lower Upper


136 100

137 10.9 8.8 13.2

54 10.5 5.0 7.4#

68 5.4 4.4 6.6

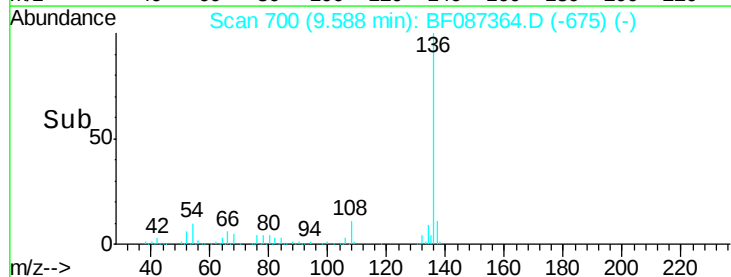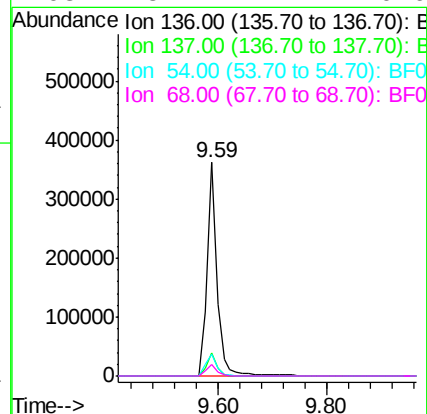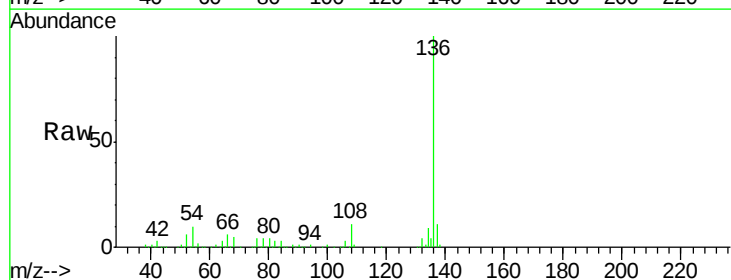

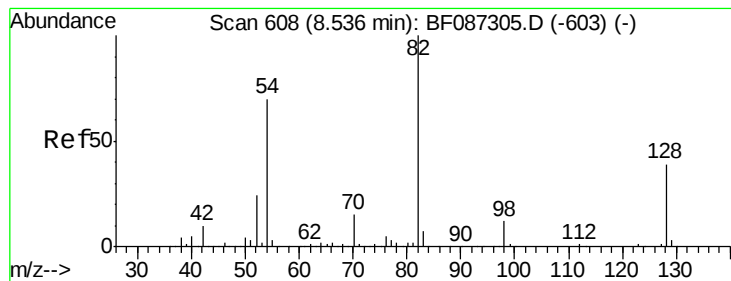

#23

Nitrobenzene-d5

Concen: 94.19 ng

RT: 8.47 min Scan# 602

Delta R.T. -0.02 min

Lab File: BF087364.D

Acq: 25 May 2016 5:51

Instrument :

BNA_F

ClientSampleId :

CHS-STA-1685(0-4)


Tot Ion: 82 Resp: 858761

Ion Ratio Lower Upper

82 100

128 37.9 40.6 61.0#




54 70.8 38.1 57.1#

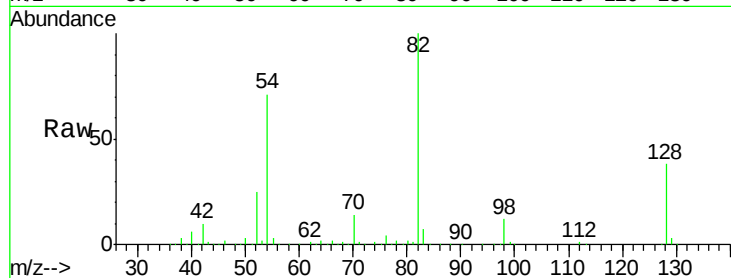

Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0

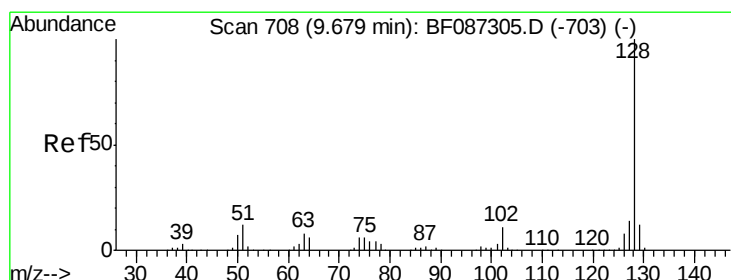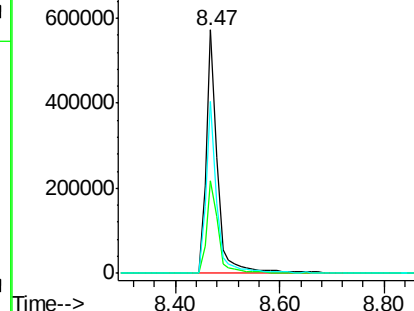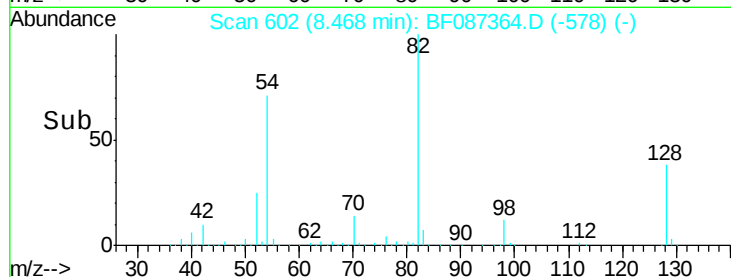

#31

Naphthalene

Concen: 5.85 ng

RT: 9.62 min Scan# 703

Delta R.T. -0.01 min

Lab File: BF087364.D

Acq: 25 May 2016 5:51


Tgt Ion: 128 Resp: 134604

Ion Ratio Lower Upper

128 100

129 11.0 8.6 13.0



127 12.7 10.8 16.2

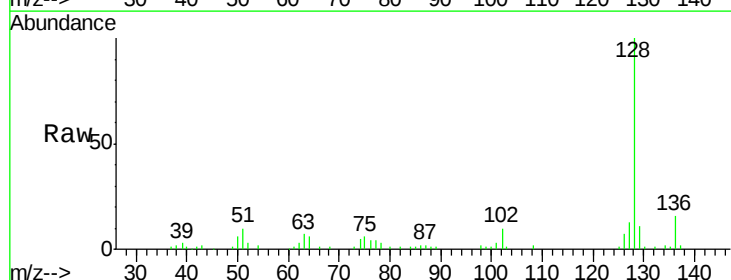


Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E



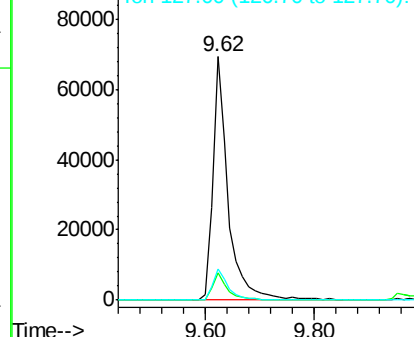
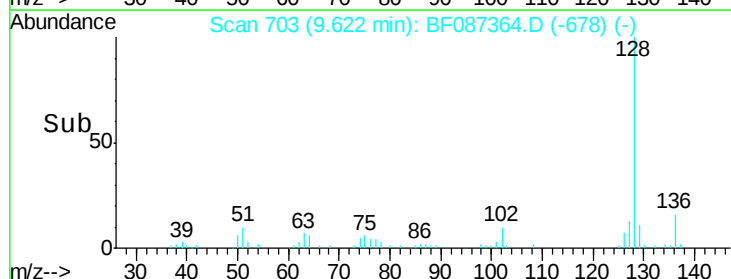


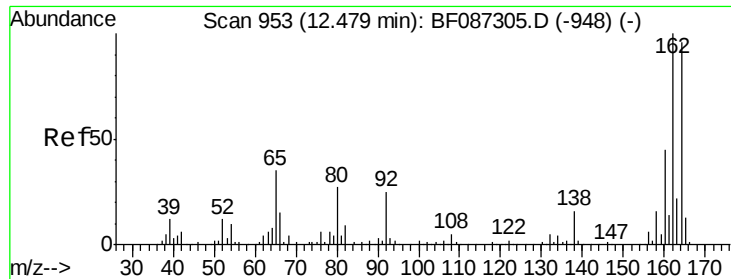

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 12.41 min Scan# 947
 Delta R.T. -0.01 min
 Lab File: BF087364.D
 Acq: 25 May 2016 5:51




Instrument :
 BNA_F
 ClientSampleId :
 CHS-STA-1685(0-4)


Tot Ion:164 Resp: 221162
 Ion Ratio Lower Upper
 164 100
 162 102.3 82.8 124.2
 160 46.4 36.9 55.3

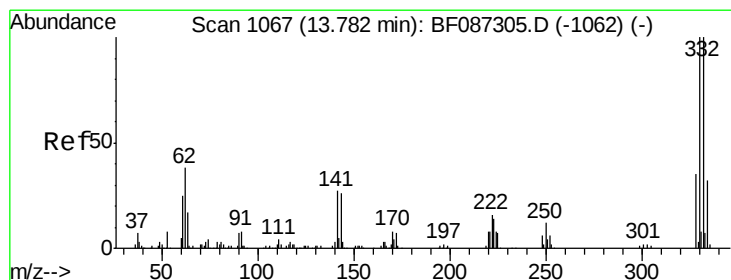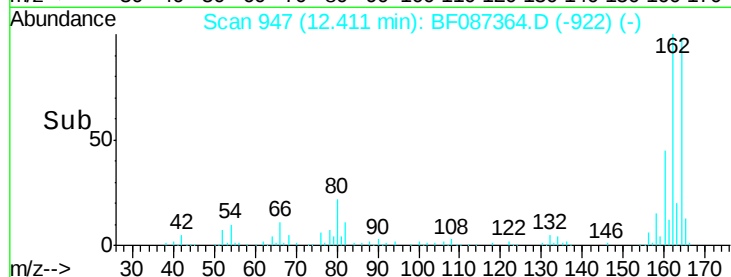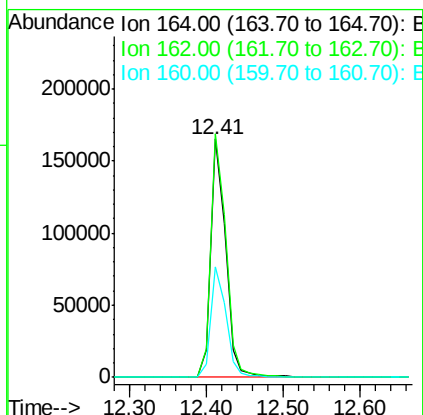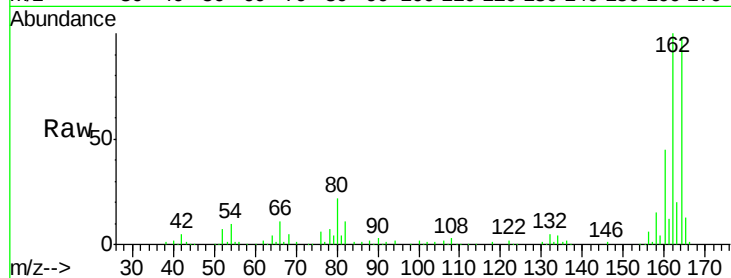

#41
 2,4,6-Tribromophenol
 Concen: 164.70 ng
 RT: 13.71 min Scan# 1061
 Delta R.T. -0.01 min
 Lab File: BF087364.D
 Acq: 25 May 2016 5:51

Tgt Ion:330 Resp: 350039
 Ion Ratio Lower Upper
 330 100
 332 95.5 79.0 118.4
 141 43.4 31.2 46.8


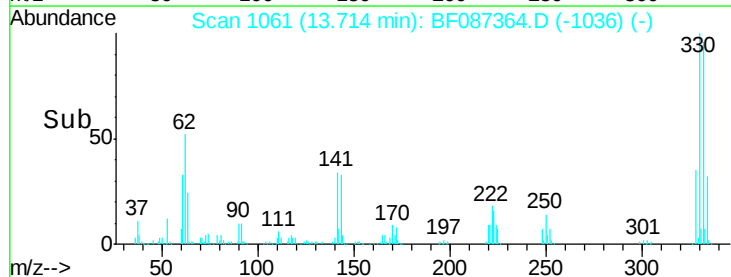
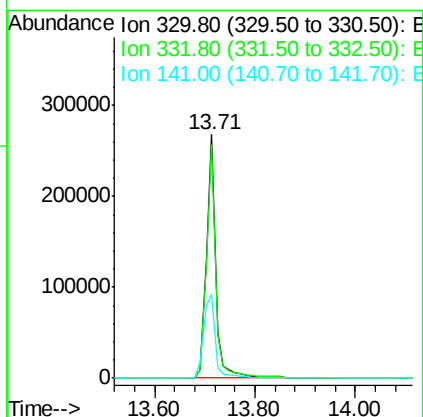
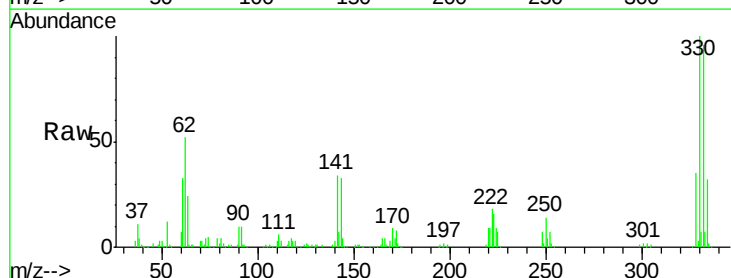


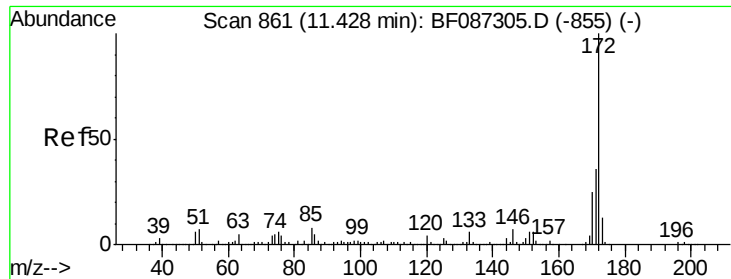

#44
 2-Fluorobiphenyl
 Concen: 97.26 ng
 RT: 11.37 min Scan# 856
 Delta R.T. -0.01 min
 Lab File: BF087364.D
 Acq: 25 May 2016 5:51




Instrument :
 BNA_F
 ClientSampleId :
 CHS-STA-1685(0-4)


Tot Ion:172 Resp: 1525826
 Ion Ratio Lower Upper
 172 100
 171 36.0 29.0 43.6
 170 24.1 19.8 29.8

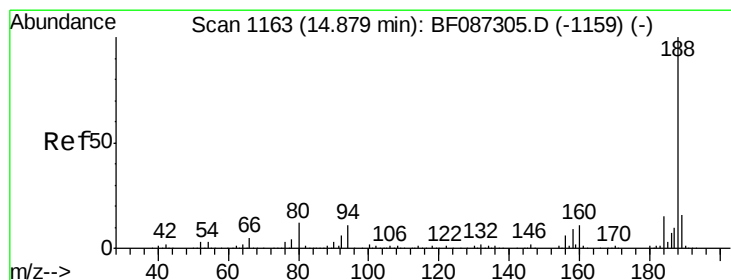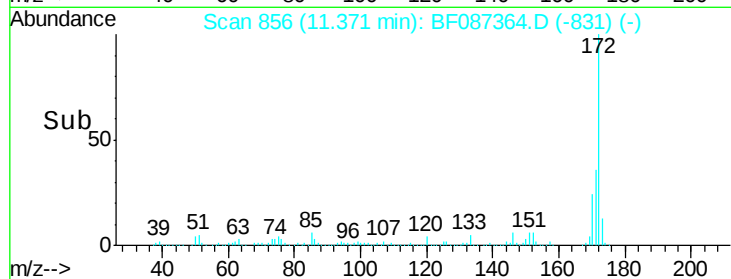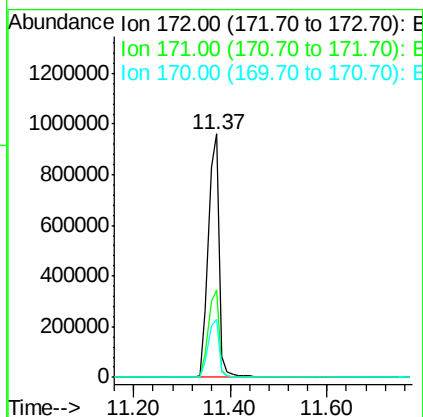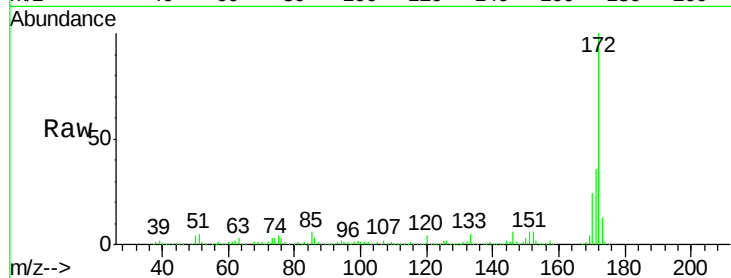

#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 14.82 min Scan# 1158
 Delta R.T. 0.00 min
 Lab File: BF087364.D
 Acq: 25 May 2016 5:51

Tgt Ion:188 Resp: 453187
 Ion Ratio Lower Upper
 188 100
 94 8.3 6.8 10.2
 80 8.8 7.1 10.7

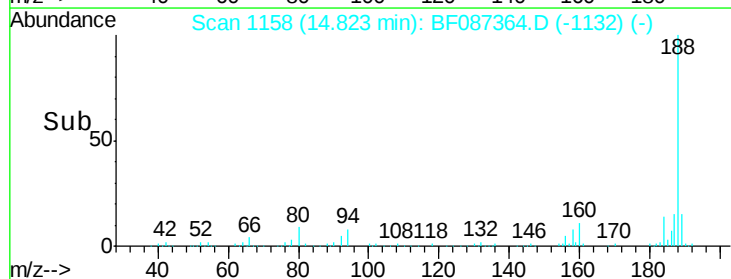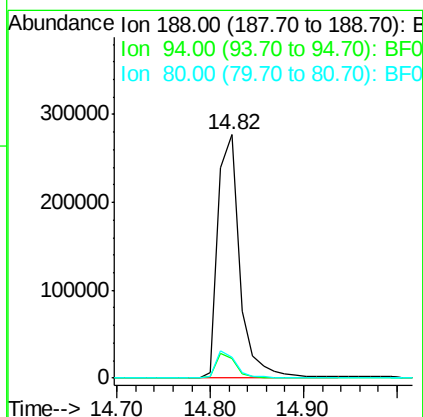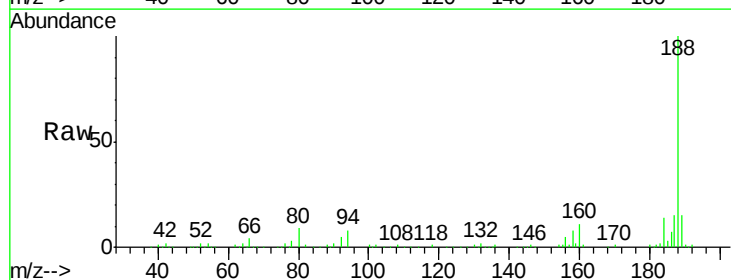

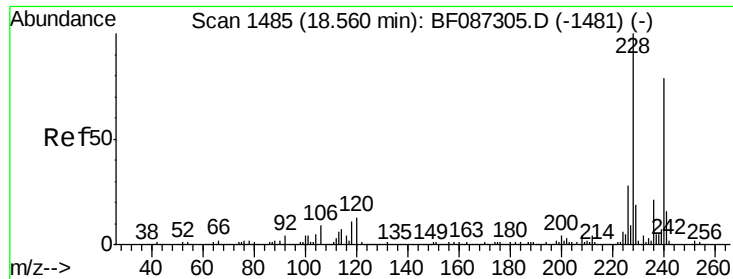

#75

Chrysene-d12

Concen: 20.00 ng

RT: 18.50 min Scan# 1480

Delta R.T. -0.01 min

Lab File: BF087364.D

Acq: 25 May 2016 5:51

Instrument :

BNA_F

ClientSampleId :

CHS-STA-1685(0-4)


Tot Ion:240 Resp: 380664

Ion Ratio Lower Upper

240 100

120 13.1 11.2 16.8




236 26.5 21.2 31.8

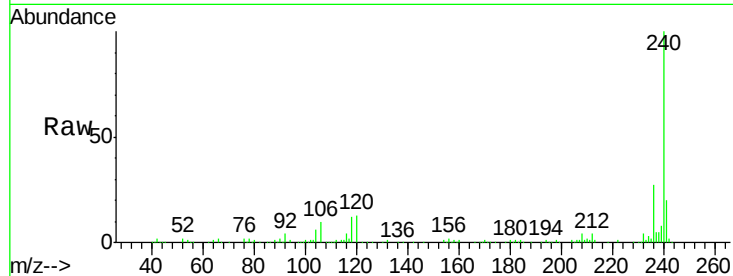

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

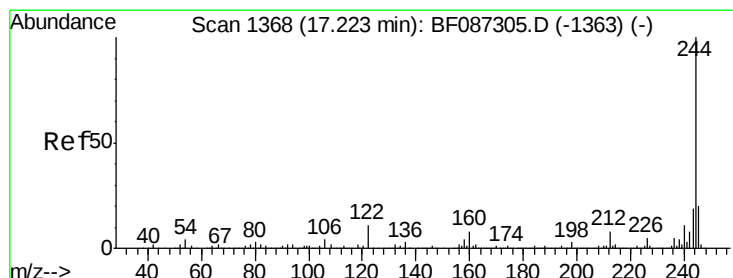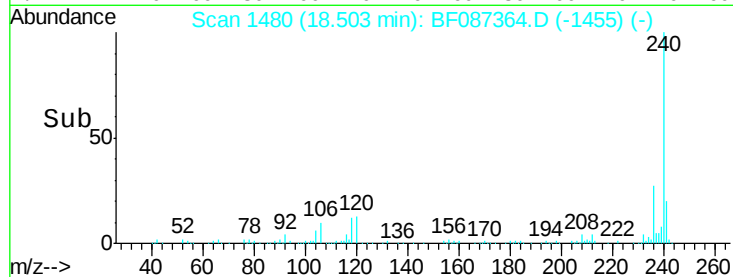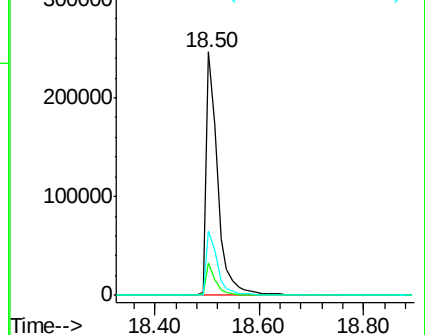

#78

Terphenyl-d14

Concen: 89.28 ng

RT: 17.17 min Scan# 1363

Delta R.T. -0.01 min

Lab File: BF087364.D

Acq: 25 May 2016 5:51


Tgt Ion:244 Resp: 1598544

Ion Ratio Lower Upper

244 100

212 7.9 6.2 9.2



122 13.5 12.0 18.0



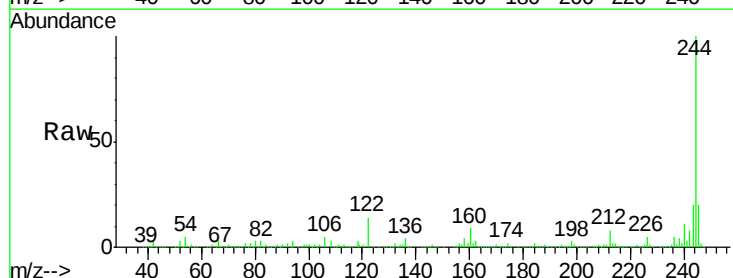


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

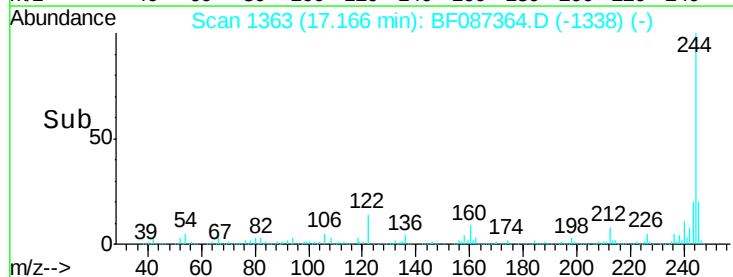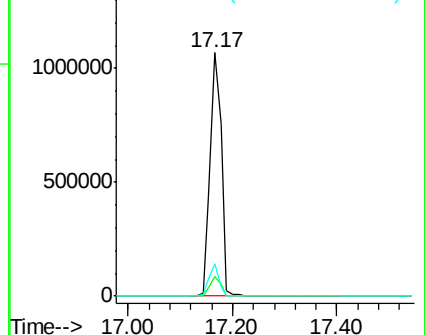

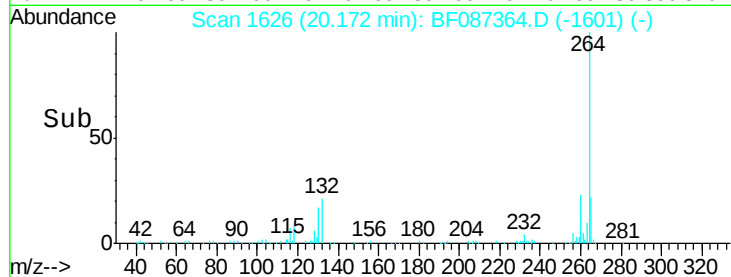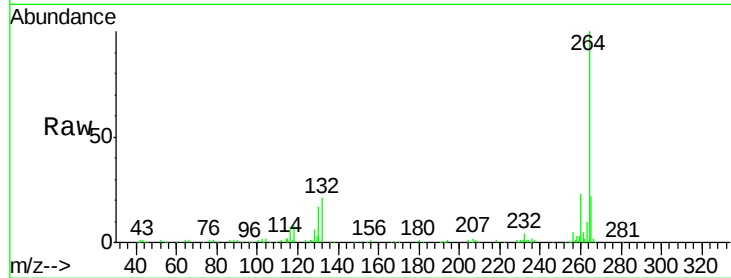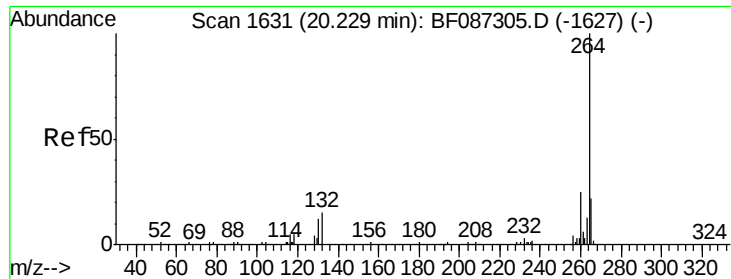

#86

Pervlene-d12

Concen: 20.00 ng

RT: 20.17 min Scan# 1626

Delta R.T. -0.01 min

Lab File: BF087364.D

Acq: 25 May 2016 5:51

Instrument :

BNA_F

ClientSampleId :

CHS-STA-1685(0-4)

Tot Ion:264 Resp: 272743

Ion Ratio Lower Upper

264 100

260 23.5 19.5 29.3

265 21.8 17.3 25.9

