


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052416\
 Data File : BF087344.D
 Acq On : 24 May 2016 18:38
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 25 16:26:52 2016

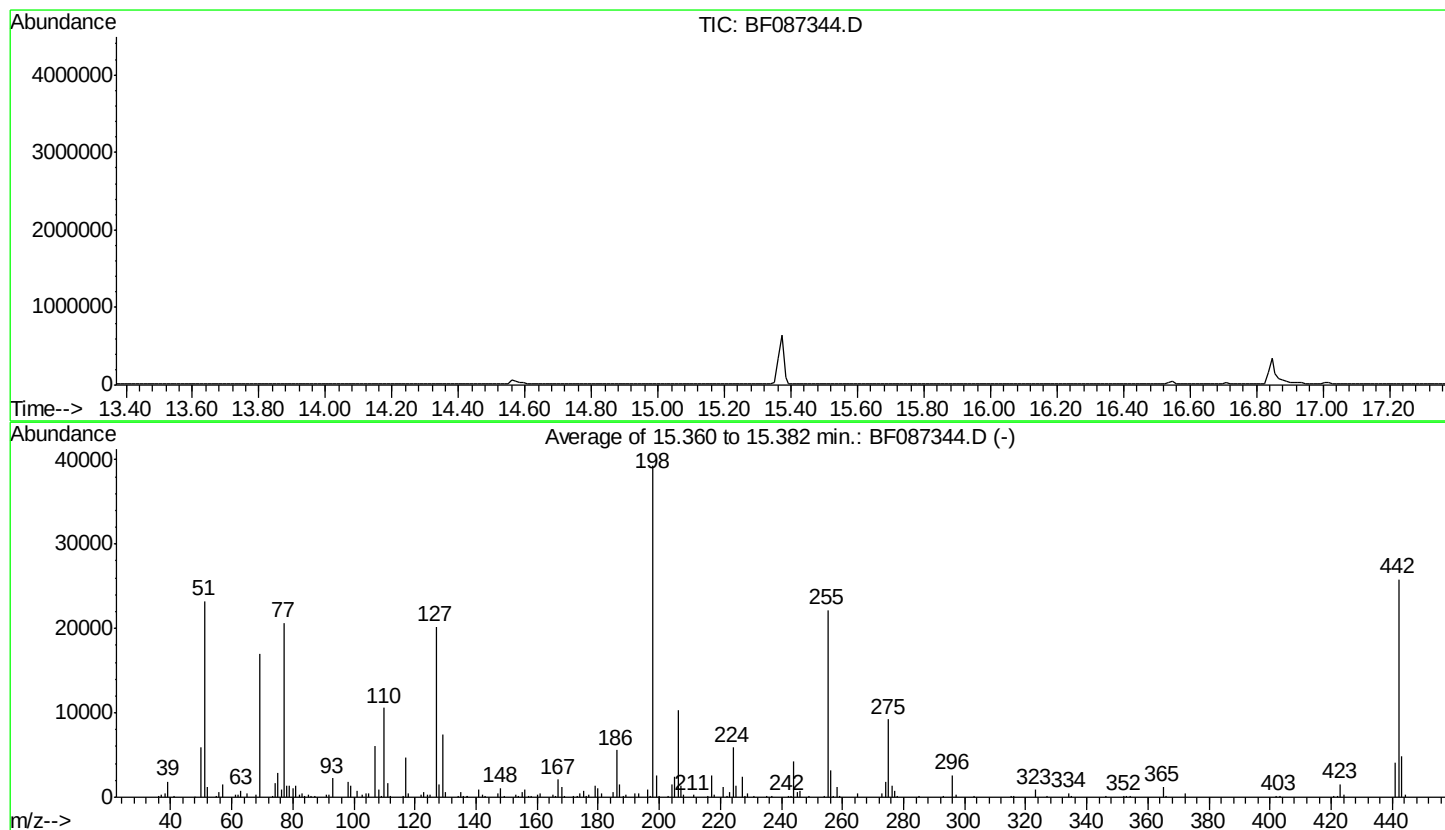

AutoFind: Scans 1205, 1206, 1207; Background Corrected with Scan 1201

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.1	23224	PASS
68	69	0.00	2	1.9	329	PASS
69	198	0.00	100	43.4	17066	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.5	20244	PASS
197	198	0.00	2	0.5	204	PASS
198	198	100	100	100.0	39296	PASS
199	198	5	9	6.5	2570	PASS
275	198	10	60	23.5	9229	PASS
365	198	1	100	3.1	1218	PASS
441	442	0.01	24	16.1	4170	PASS
442	198	50	100	65.8	25849	PASS
443	442	15	24	18.9	4876	PASS