


Data Path : Z:\HPCHEM1\BNA F\Data\BF052417\
 Data File : BF095382.D
 Acq On : 24 May 2017 11:24
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 18 17:07:53 2017

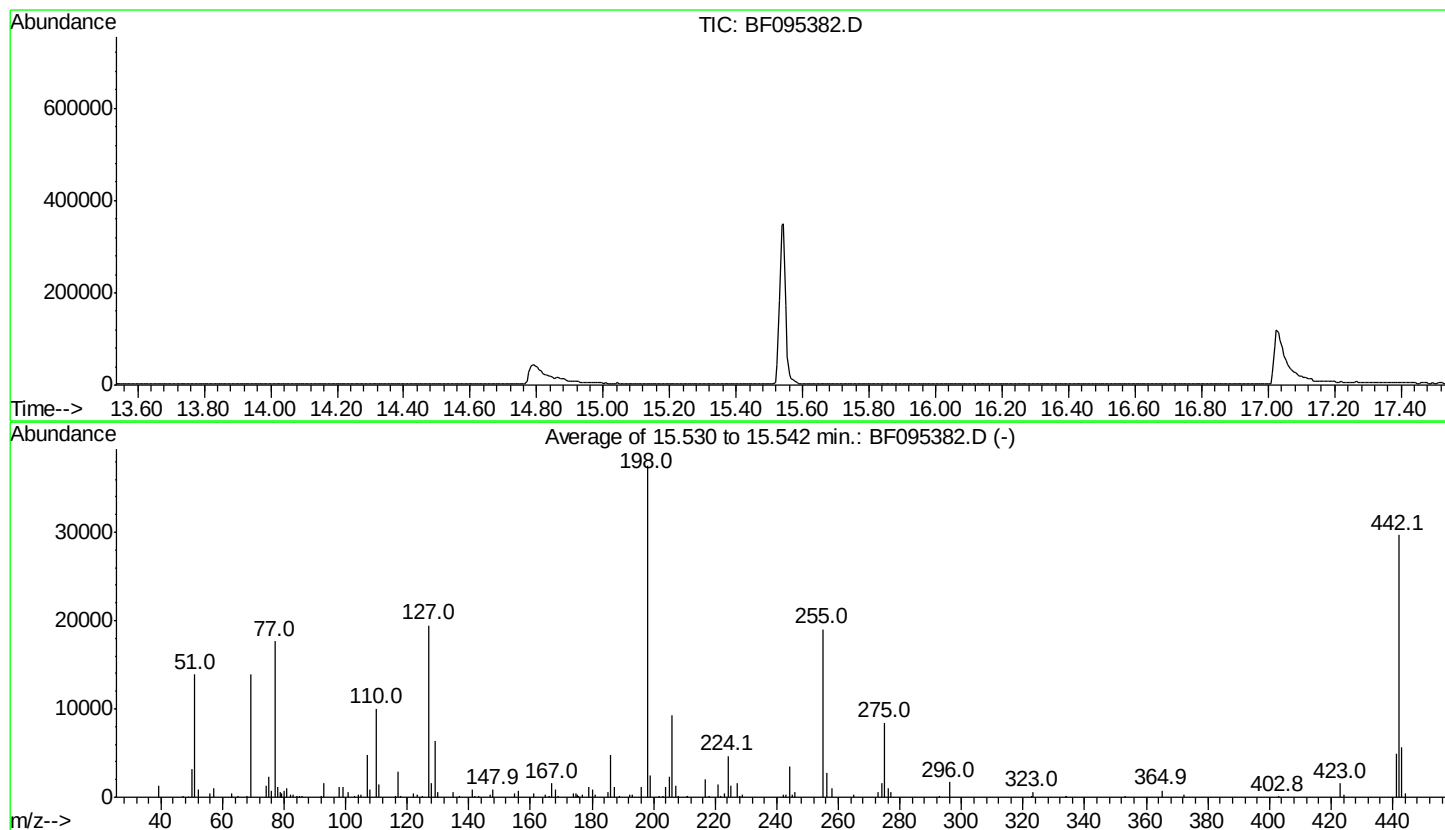

AutoFind: Scans 2311, 2312, 2313; Background Corrected with Scan 2306

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.0	13884	PASS
68	69	0.00	2	0.8	109	PASS
69	198	0.00	100	37.2	13974	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.8	19463	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	37538	PASS
199	198	5	9	6.4	2403	PASS
275	198	10	60	22.5	8446	PASS
365	198	1	100	2.0	746	PASS
441	442	0.01	24	16.4	4878	PASS
442	198	50	100	79.0	29662	PASS
443	442	15	24	18.9	5602	PASS