


Data Path : Z:\HPCHEM1\BNA F\Data\BF052417\
 Data File : BF095405.D
 Acq On : 25 May 2017 1:22
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampled :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 18 17:07:53 2017

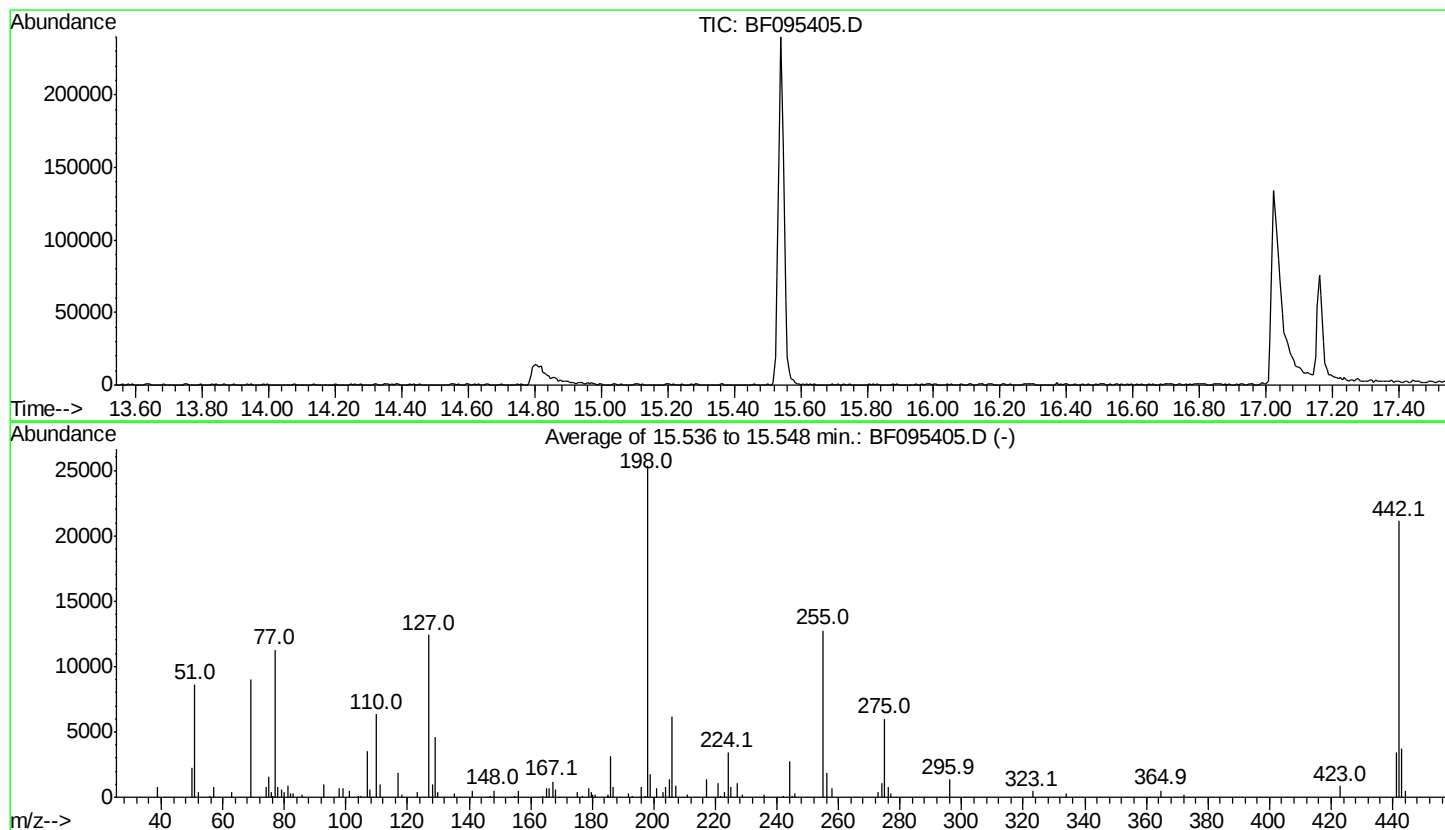

AutoFind: Scans 2312, 2313, 2314; Background Corrected with Scan 2306

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.9	8593	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.5	9000	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.9	12403	PASS
197	198	0.00	2	0.4	100	PASS
198	198	100	100	100.0	25360	PASS
199	198	5	9	6.9	1762	PASS
275	198	10	60	23.6	5983	PASS
365	198	1	100	2.1	540	PASS
441	442	0.01	24	16.1	3403	PASS
442	198	50	100	83.3	21135	PASS
443	442	15	24	17.8	3770	PASS