
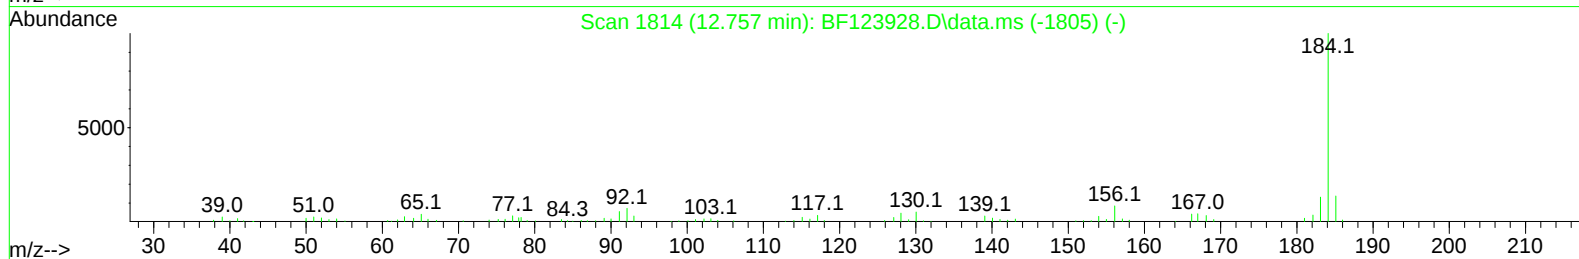
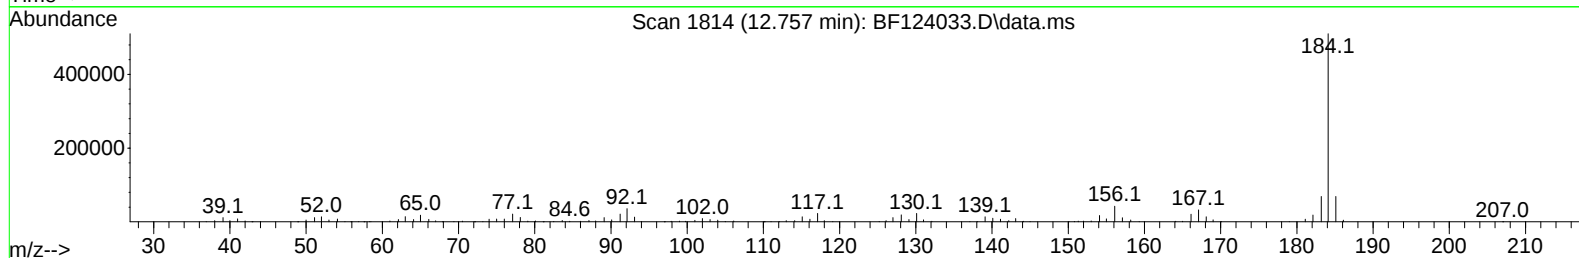


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052421\
Data File : BF124033.D
Acq On : 24 May 2021 11:16
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 24 13:24:10 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 19:05:57 2021
Response via : Initial Calibration

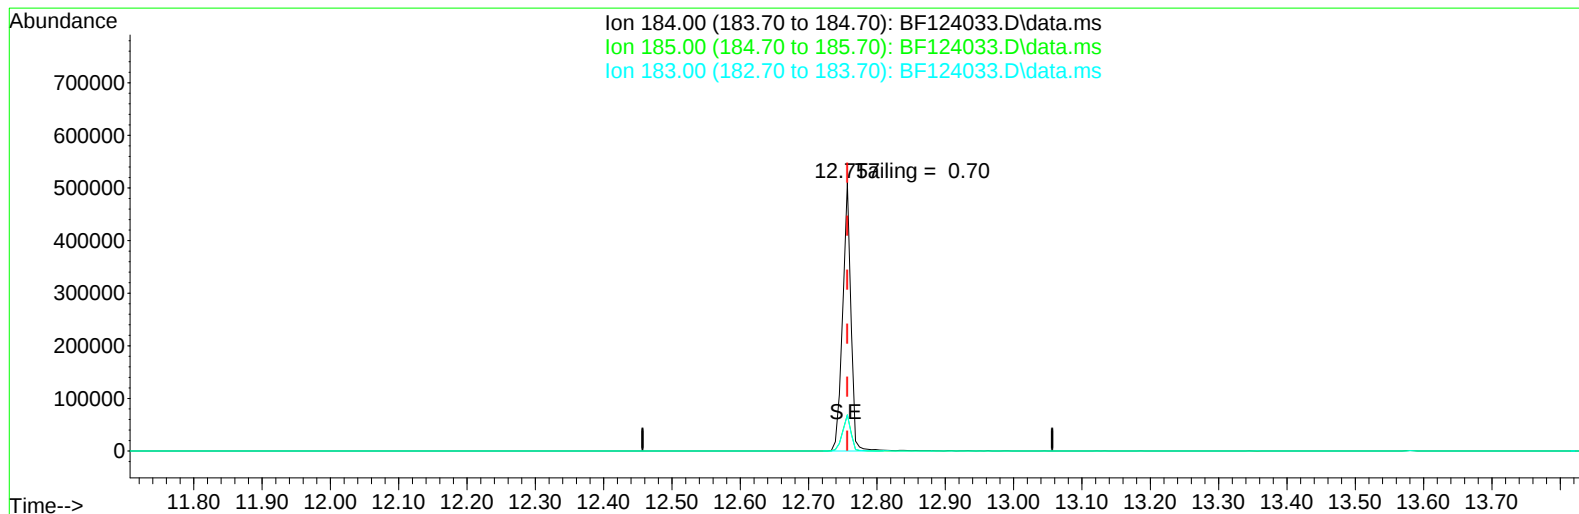

TIC: BF124033.D\data.ms

(77) Benzidine




12.757min (-0.000) 0.00 ng

response 425313

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.47
183.00	9.80	13.51#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052421\
Data File : BF124033.D
Acq On : 24 May 2021 11:16
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 24 13:24:10 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 19:05:57 2021
Response via : Initial Calibration

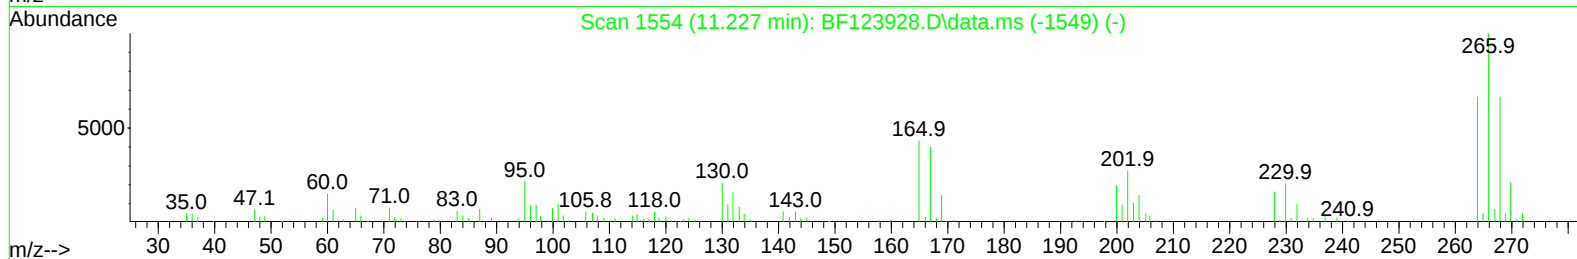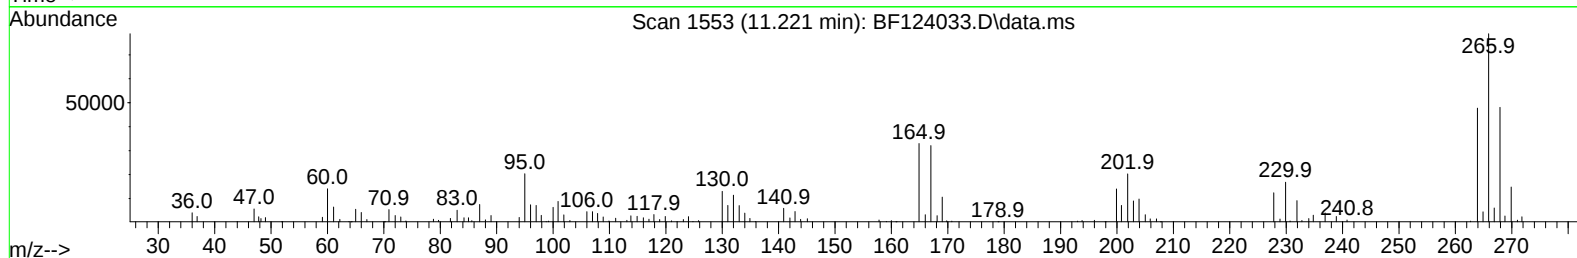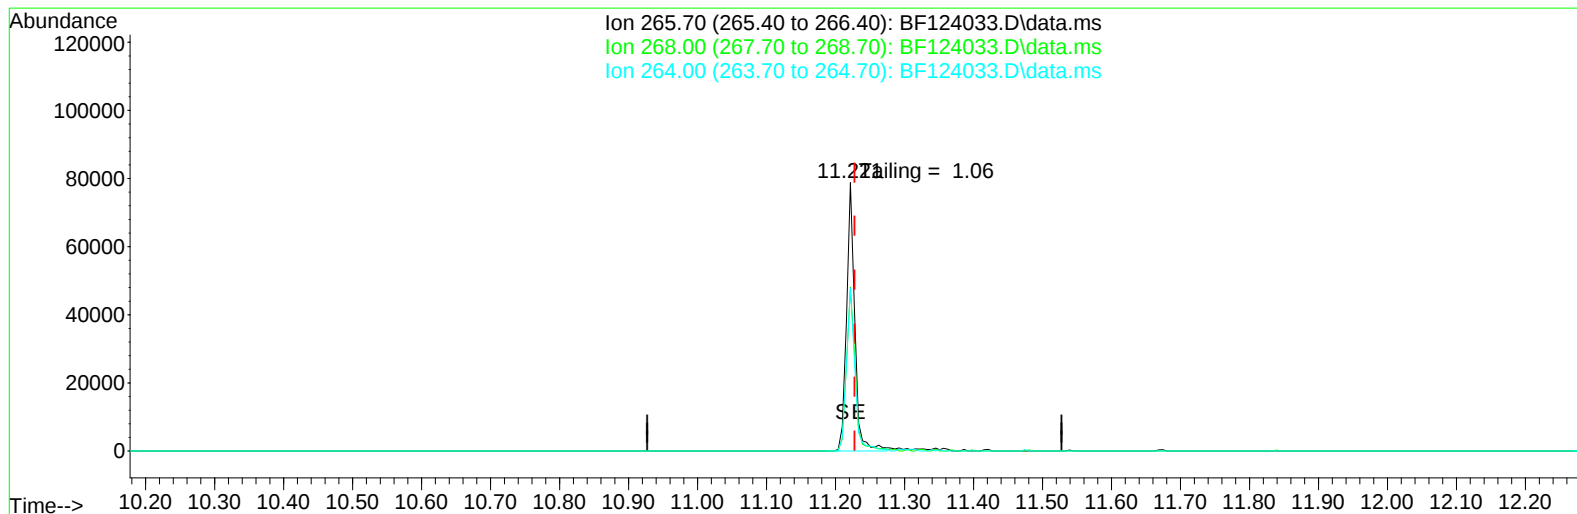

TIC: BF124033.D\data.ms

(70) Pentachlorophenol (C)

11.221min (-0.006) 22128.89 ng

response 64287

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	60.97
264.00	65.70	60.56
0.00	0.00	0.00