

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052421\
 Data File : BF124036.D
 Acq On : 24 May 2021 14:24
 Operator : JU/CG
 Sample : PB136602BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB136602BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124036.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.269	22	31	37	rVB	60652	85389	2.85%	0.502%
2	5.522	578	584	587	rBV	2173885	2352405	78.45%	13.832%
3	6.522	747	754	757	rBV	2088740	2316991	77.27%	13.623%
4	6.892	813	817	820	rVB	493901	425444	14.19%	2.502%
5	7.451	906	912	915	rBV	1362481	1589665	53.02%	9.347%
6	8.175	1030	1035	1038	rBV	622149	543596	18.13%	3.196%
7	9.251	1212	1218	1221	rBV	3171355	2766636	92.27%	16.267%
8	9.927	1329	1333	1337	rBV	693863	618891	20.64%	3.639%
9	10.722	1463	1468	1471	rBV	1978511	1763775	58.82%	10.371%
10	11.416	1582	1586	1590	rBV	743602	627175	20.92%	3.688%
11	13.010	1852	1857	1860	rBV	3519317	2998479	100.00%	17.631%
12	14.063	2031	2036	2039	rBV	536860	505747	16.87%	2.974%
13	15.551	2283	2289	2294	rBV2	323262	413120	13.78%	2.429%




Sum of corrected areas: 17007313

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052421\
Data File : BF124036.D
Acq On : 24 May 2021 14:24
Operator : JU/CG
Sample : PB136602BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB136602BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

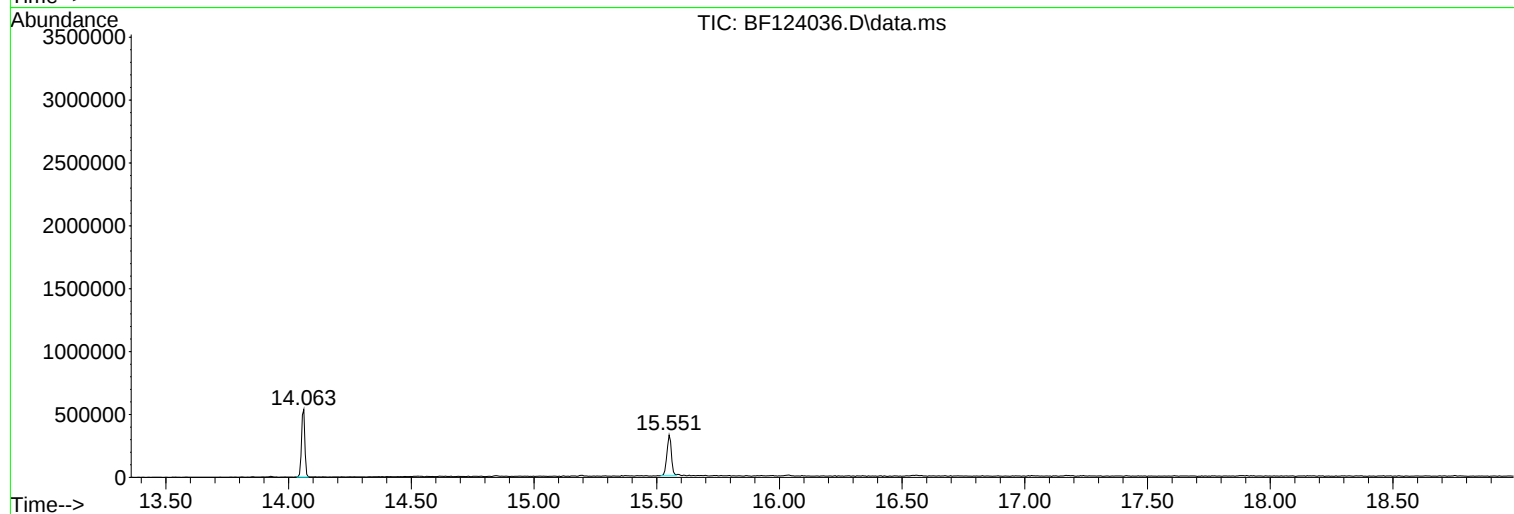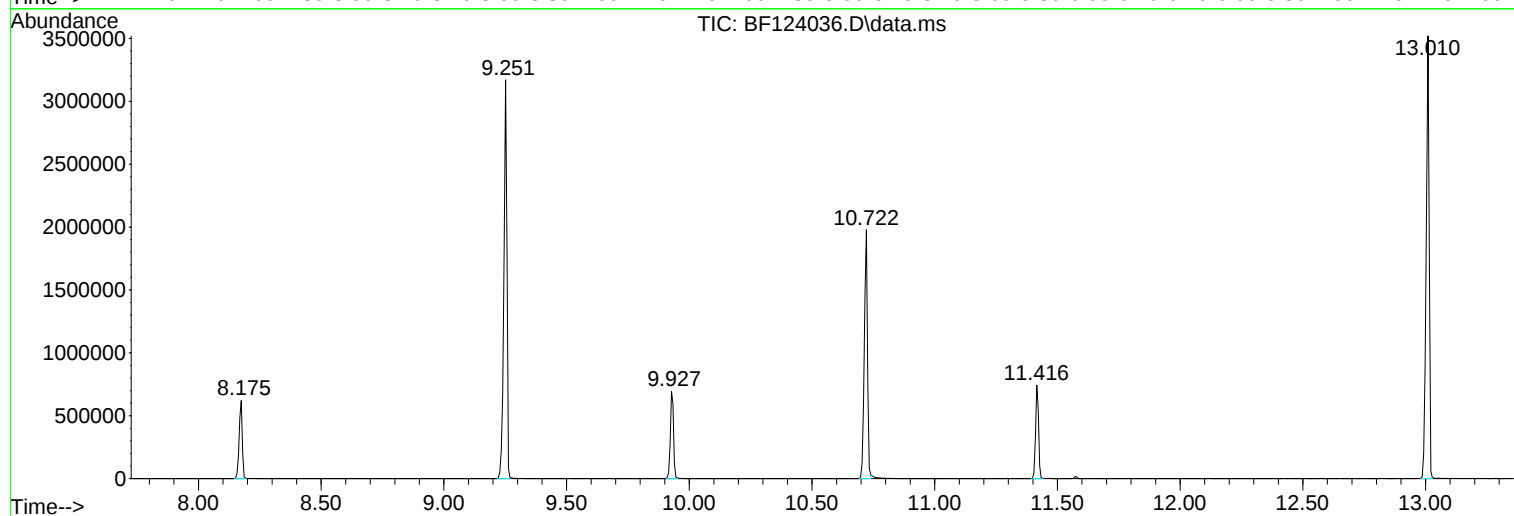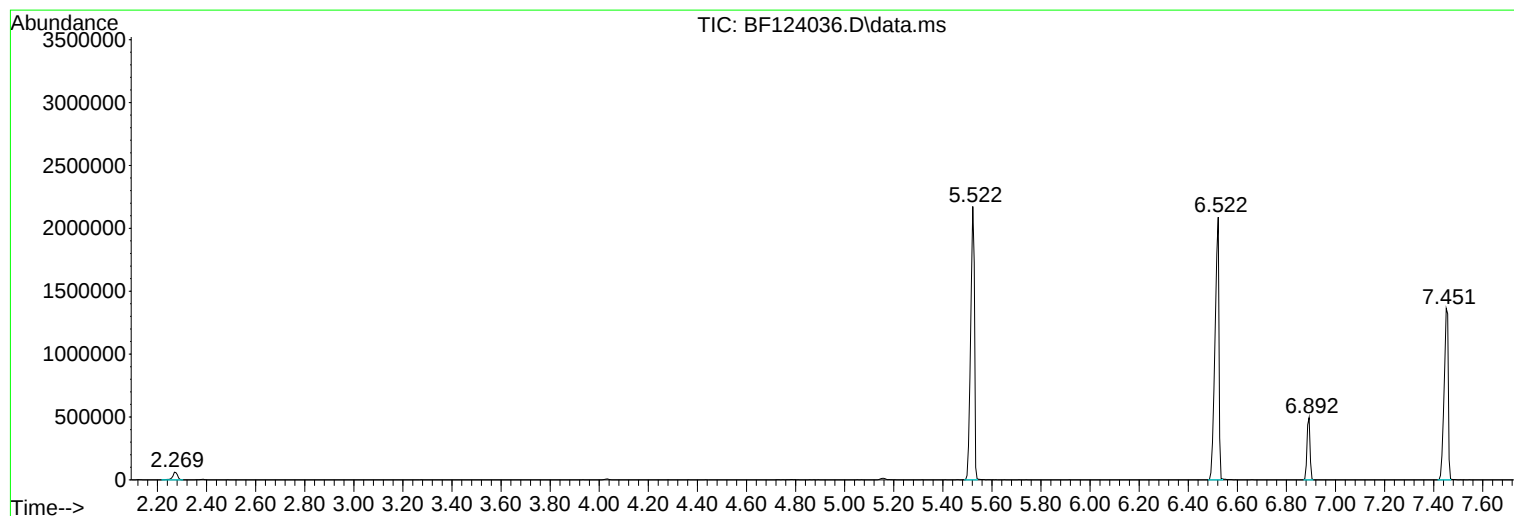

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052421\
Data File : BF124036.D
Acq On : 24 May 2021 14:24
Operator : JU/CG
Sample : PB136602BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB136602BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052421\
Data File : BF124036.D
Acq On : 24 May 2021 14:24
Operator : JU/CG
Sample : PB136602BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB136602BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------