
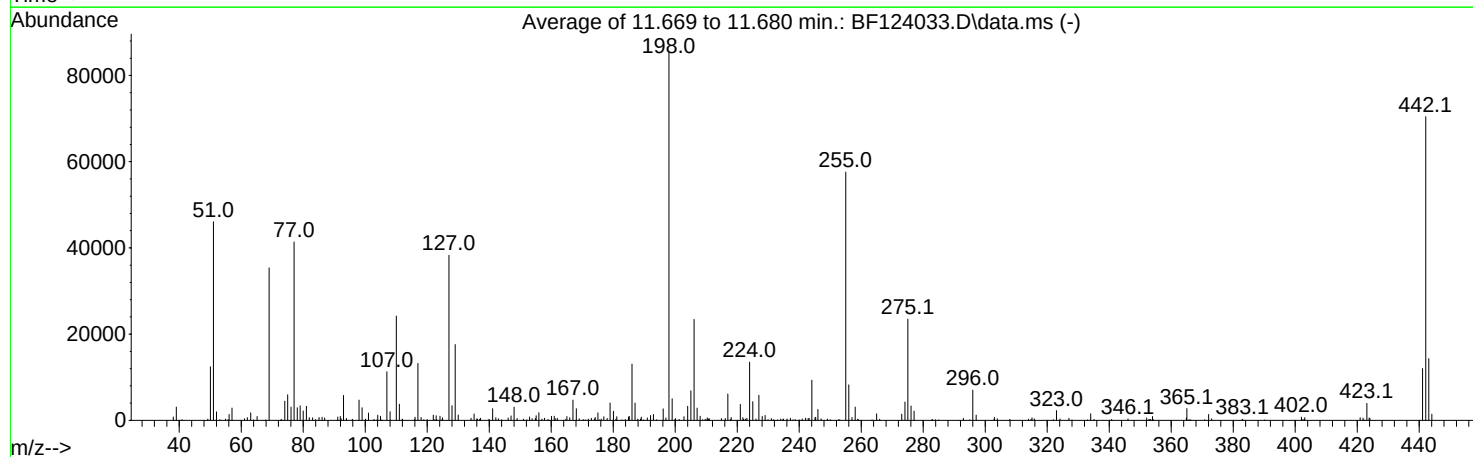


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052421\
 Data File : BF124033.D
 Acq On : 24 May 2021 11:16
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 14 19:05:57 2021

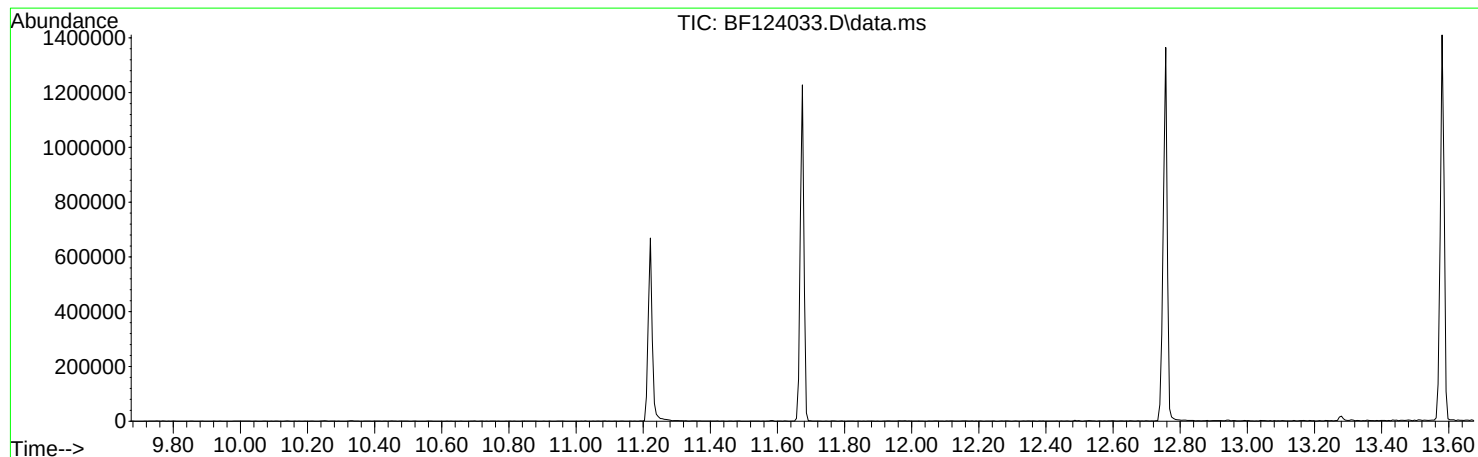

AutoFind: Scans 1629, 1630, 1631; Background Corrected with Scan 1624

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.0	46040	PASS
68	69	0.00	2	0.4	130	PASS
69	198	0.00	100	41.4	35360	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.9	38315	PASS
197	198	0.00	2	0.6	550	PASS
198	198	100	100	100.0	85323	PASS
199	198	5	9	5.9	5014	PASS
275	198	10	60	27.5	23481	PASS
365	198	1	100	3.2	2756	PASS
441	198	0.01	100	14.1	12014	PASS
442	442	50	100	100.0	70459	PASS
443	442	15	24	20.3	14329	PASS

Instrument :
BNA_F
ClientSampleId :
DFTPP

Instrument :
BNA_F
ClientSampleId :
DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/24/2021	BNA_F	<u>BF124033.D</u>
Compound Name	Response	Retention Time
DDT	203684	13.58
DDD	3347	13.28
DDE	899	12.94
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4246	207930	2.04

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052421\
Data File : BF124033.D
Acq On : 24 May 2021 11:16
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 24 13:24:10 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 19:05:57 2021
Response via : Initial Calibration

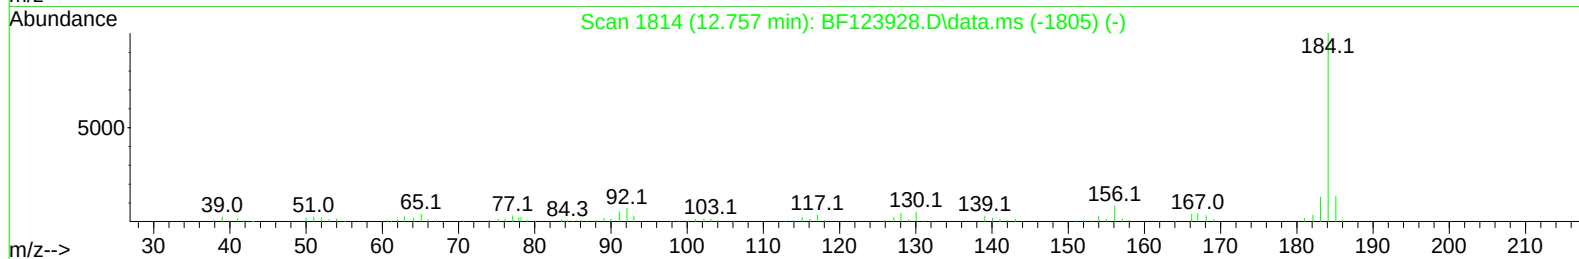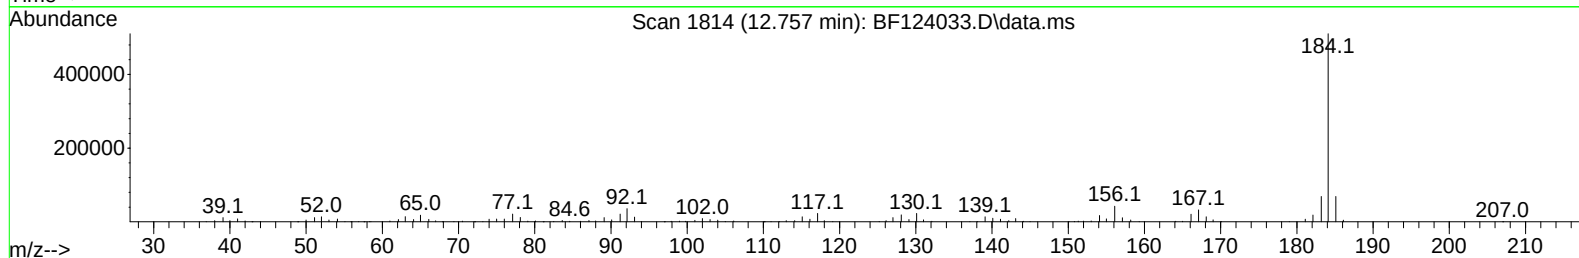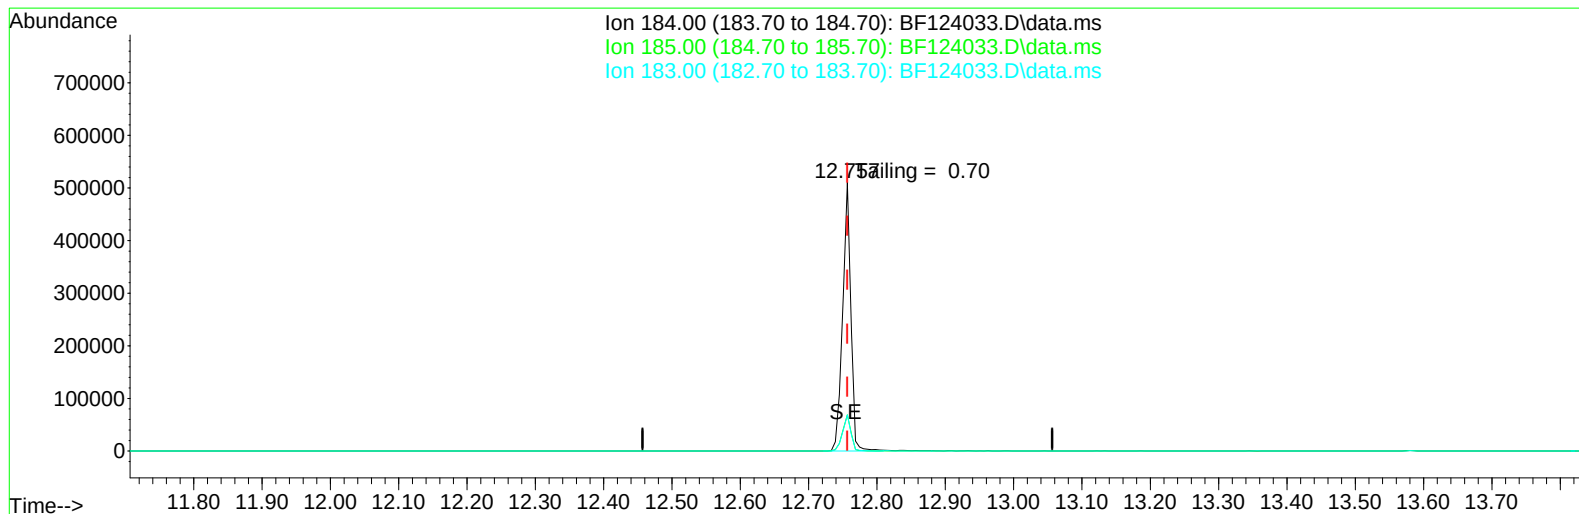

TIC: BF124033.D\data.ms

(77) Benzidine

12.757min (-0.000) 0.00 ng




response 425313

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.47
183.00	9.80	13.51#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052421\
Data File : BF124033.D
Acq On : 24 May 2021 11:16
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 24 13:24:10 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 19:05:57 2021
Response via : Initial Calibration

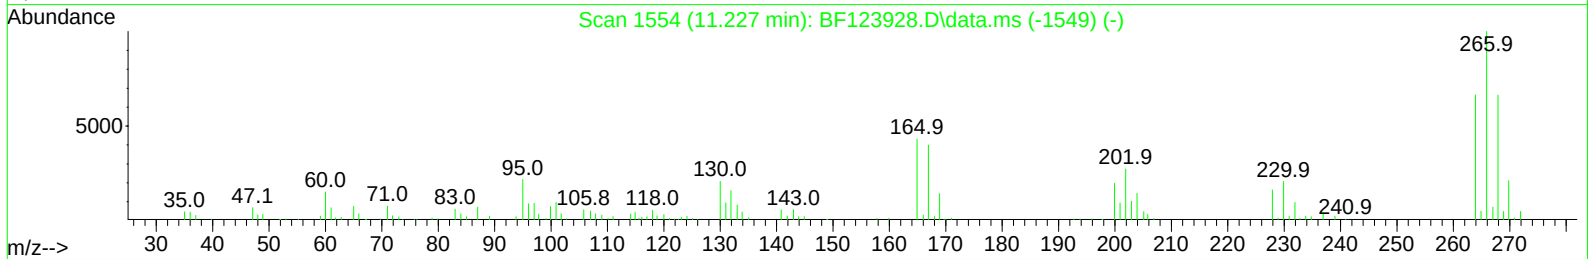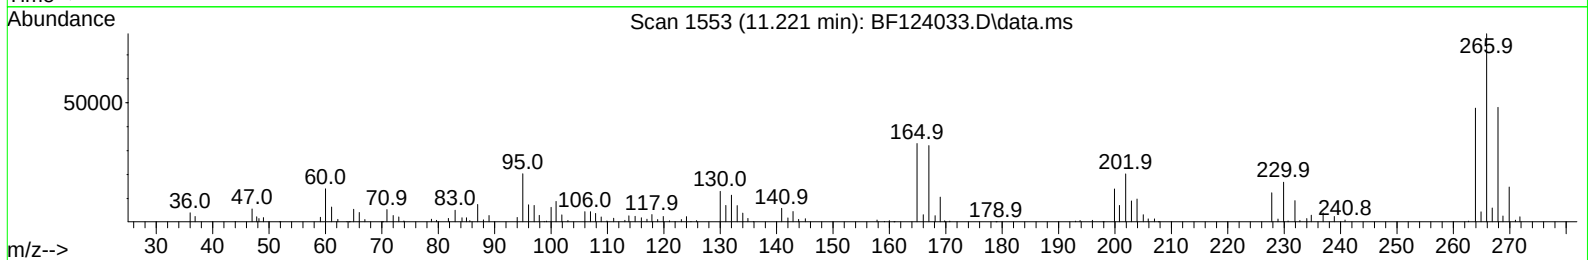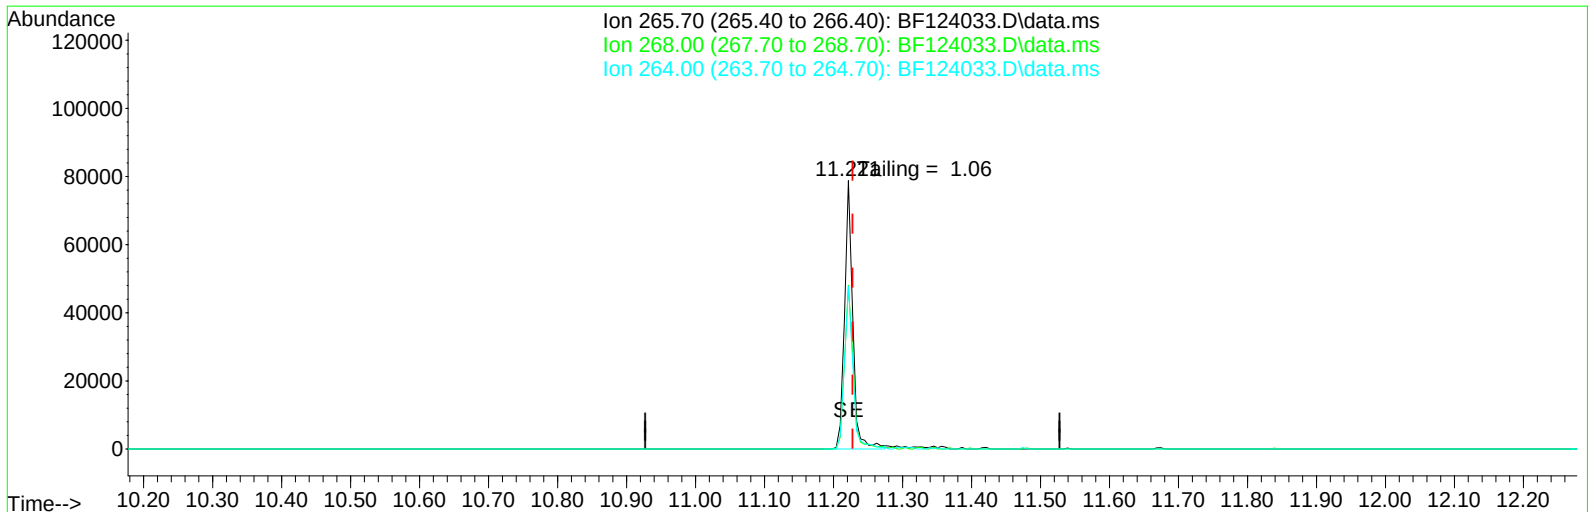

TIC: BF124033.D\data.ms

(70) Pentachlorophenol (C)

11.221min (-0.006) 22128.89 ng

response 64287

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	60.97
264.00	65.70	60.56
0.00	0.00	0.00