
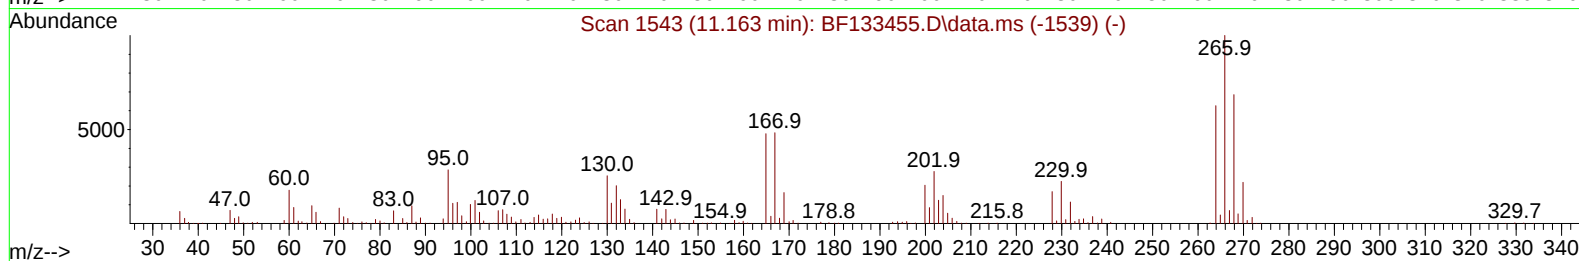
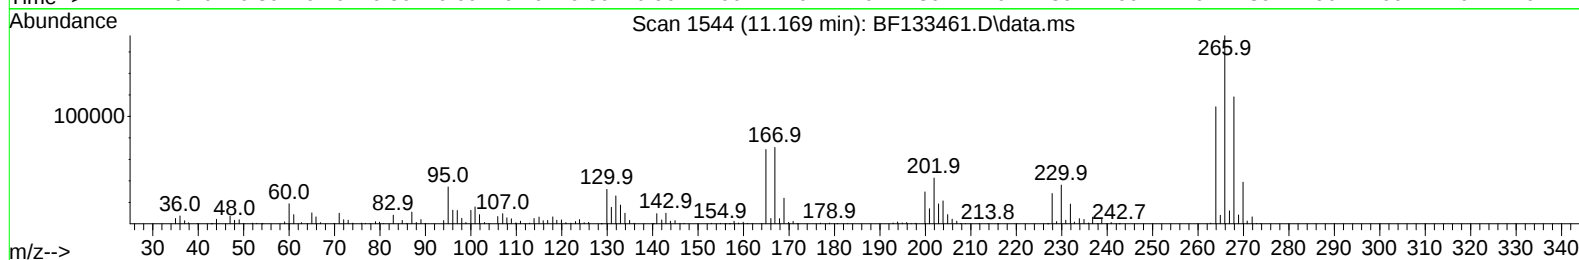


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052423\
Data File : BF133461.D
Acq On : 24 May 2023 10:10
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 24 13:47:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 24 02:41:39 2023
Response via : Initial Calibration

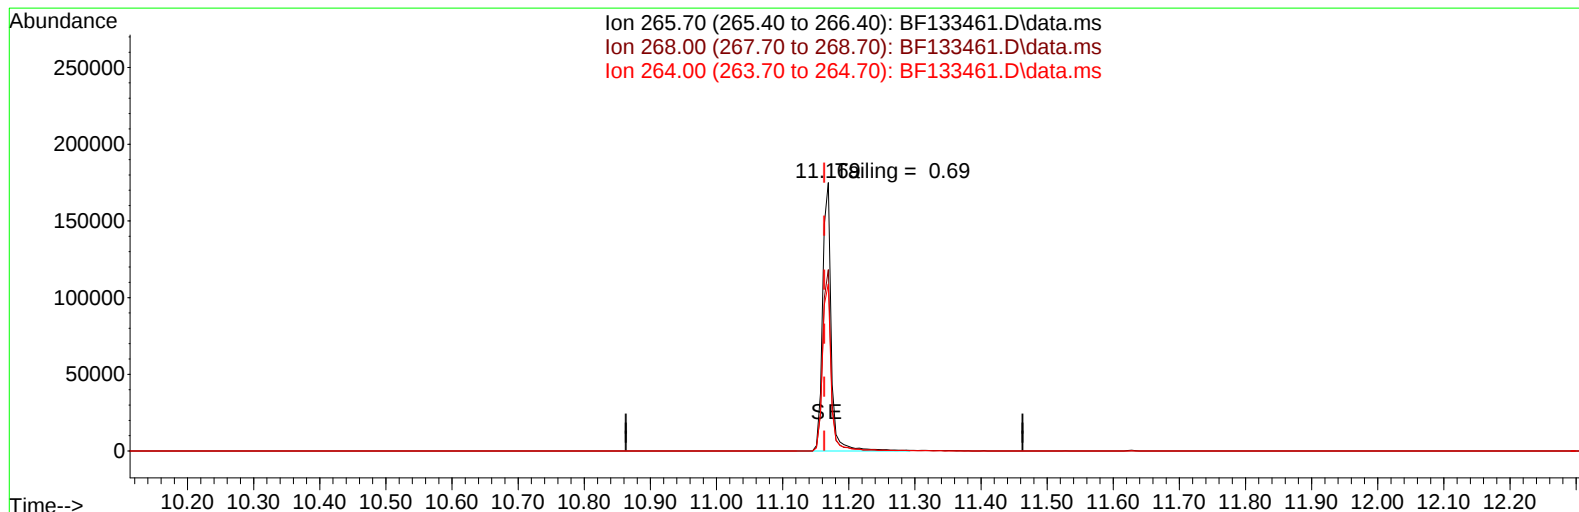

TIC: BF133461.D\data.ms

(70) Pentachlorophenol (C)




11.169min (+ 0.006) 470188.66 ng

response 158584

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	68.50	67.53
264.00	62.70	62.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052423\
Data File : BF133461.D
Acq On : 24 May 2023 10:10
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 24 13:47:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 24 02:41:39 2023
Response via : Initial Calibration

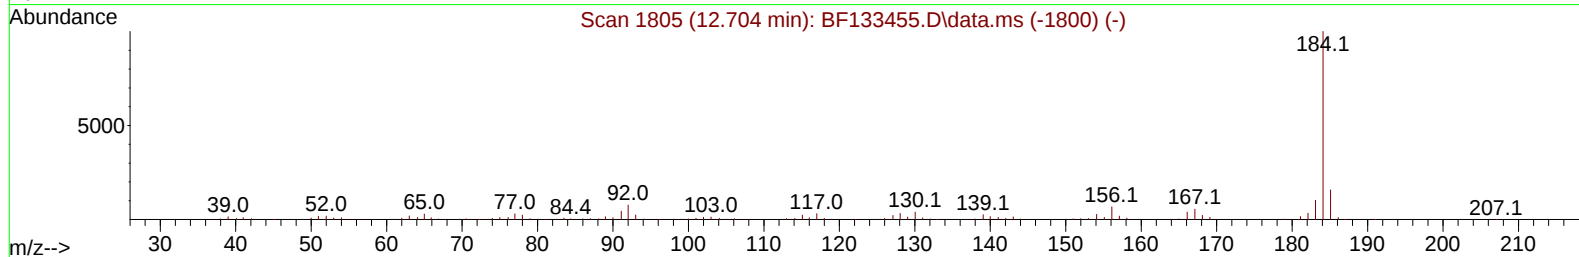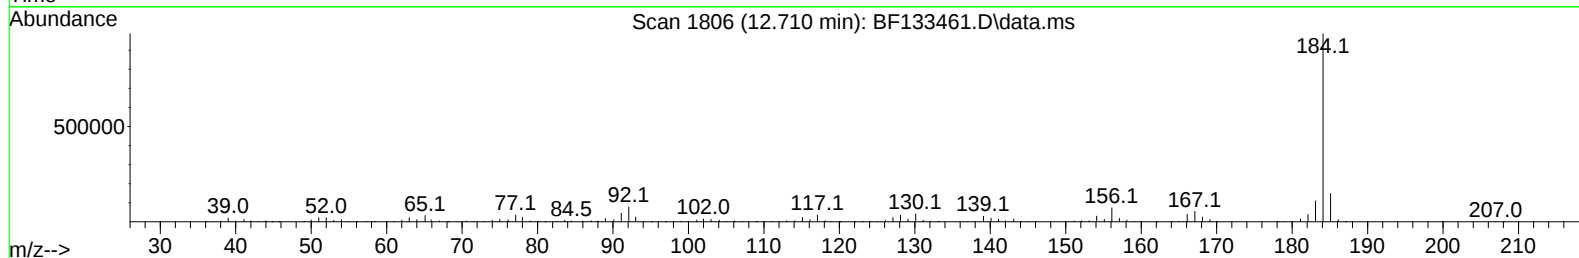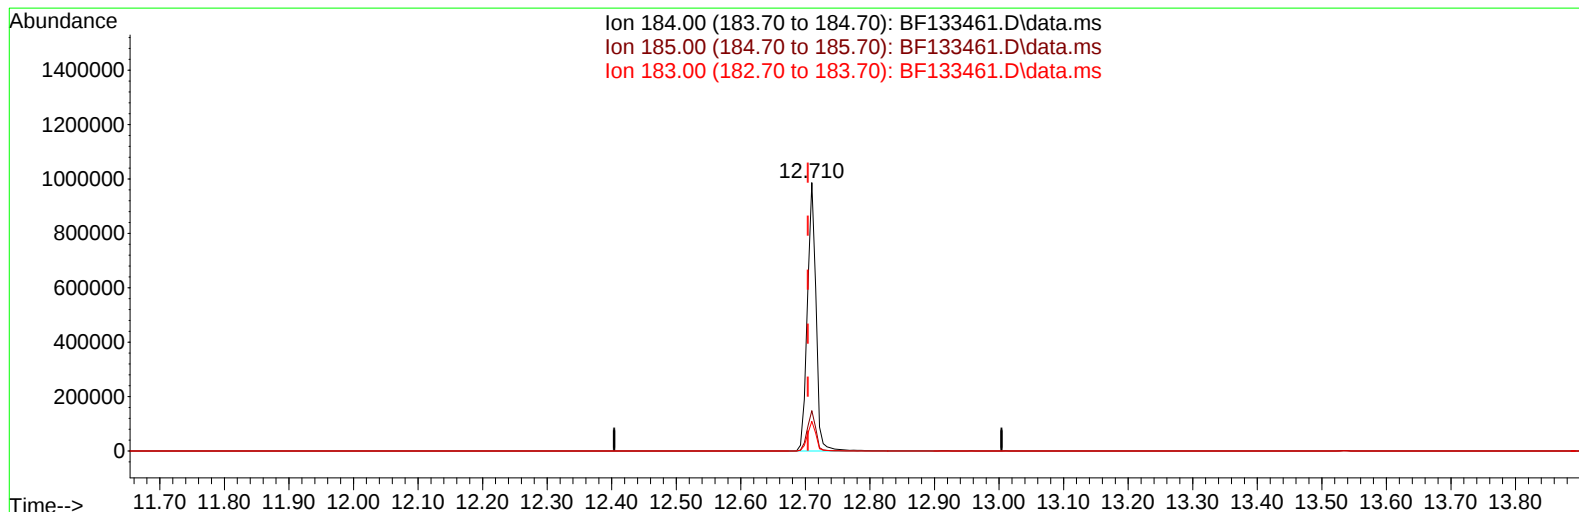

TIC: BF133461.D\data.ms

(77) Benzidine**12.710min (+ 0.006) 0.00 ng****response 924409**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.80	15.02
183.00	10.20	11.07
0.00	0.00	0.00