

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052423\
 Data File : BF133466.D
 Acq On : 24 May 2023 12:47
 Operator : CG\JU
 Sample : 02891-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 290-328

Quant Time: May 24 14:23:22 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 24 02:41:39 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.839	152	103822	20.000	ng	0.00
21) Naphthalene-d8	8.122	136	397740	20.000	ng	0.00
39) Acenaphthene-d10	9.875	164	193801	20.000	ng	0.00
64) Phenanthrene-d10	11.363	188	383973	20.000	ng	0.00
76) Chrysene-d12	14.004	240	306300	20.000	ng	0.00
86) Perylene-d12	15.462	264	277045	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.457	112	723944	113.982	ng	0.01
7) Phenol-d6	6.463	99	800600	104.856	ng	0.00
23) Nitrobenzene-d5	7.404	82	608112	105.702	ng	0.00
42) 2,4,6-Tribromophenol	10.669	330	271828	151.838	ng	0.00
45) 2-Fluorobiphenyl	9.204	172	1087516	78.950	ng	0.00
79) Terphenyl-d14	12.957	244	1349321	84.224	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052423\
Data File : BF133466.D
Acq On : 24 May 2023 12:47
Operator : CG\JU
Sample : 02891-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
290-328

Quant Time: May 24 14:23:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 24 02:41:39 2023
Response via : Initial Calibration




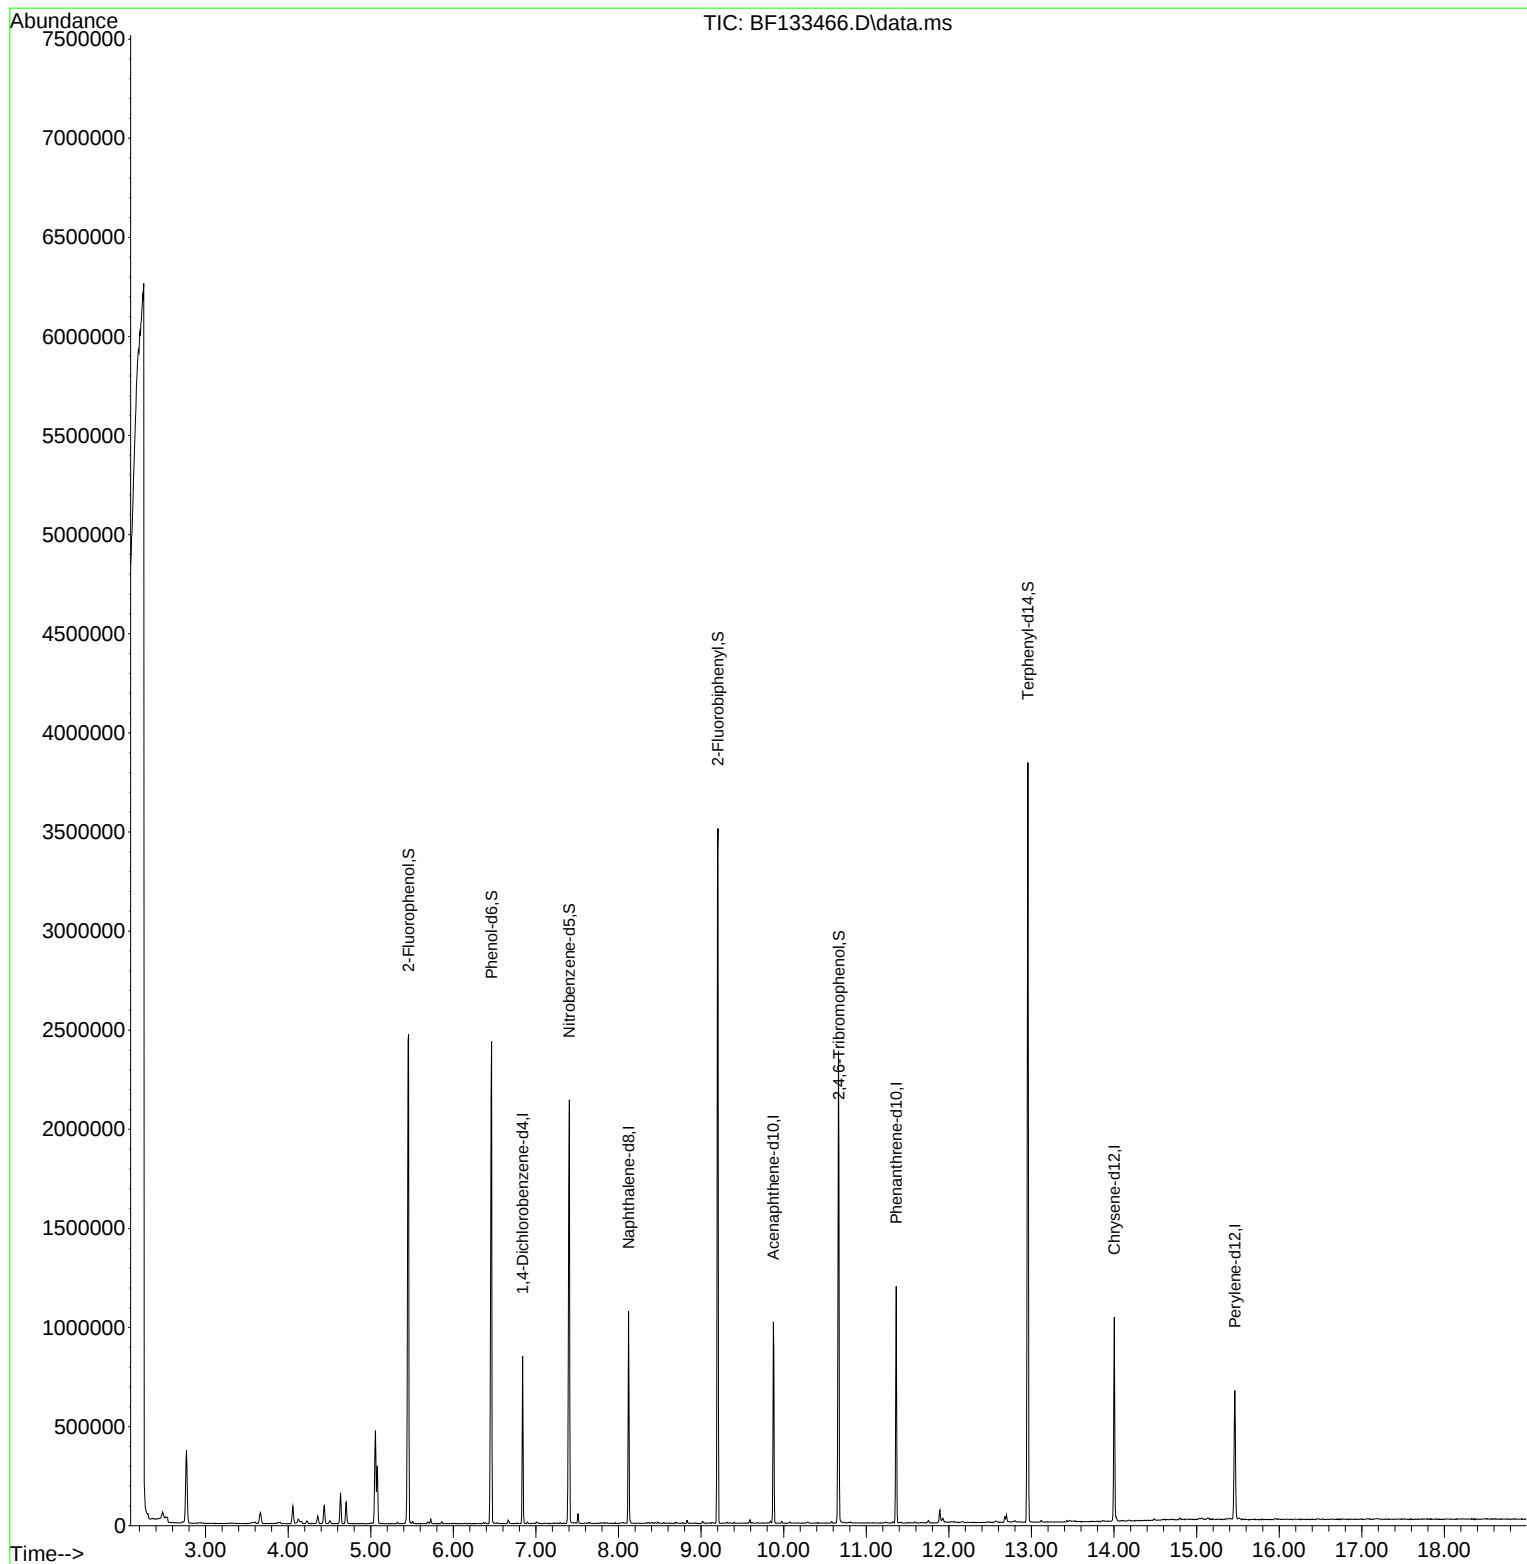


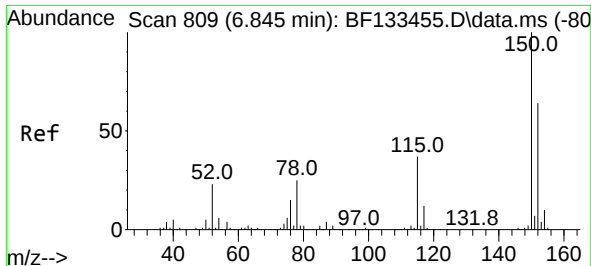

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.839 min Scan# 809
Delta R.T. -0.006 min
Lab File: BF133466.D
Acq: 24 May 2023 12:47




Instrument :
BNA_F
ClientSampleId :
290-328


Tgt Ion:152 Resp: 103822
Ion Ratio Lower Upper
152 100
150 158.7 125.6 188.4
115 60.8 47.0 70.4

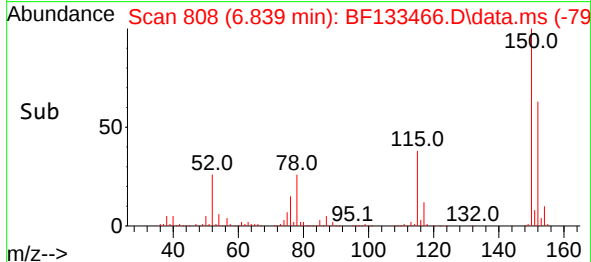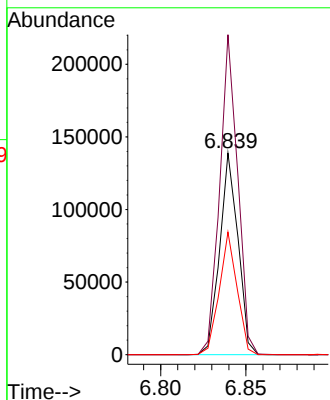

#5
2-Fluorophenol
Concen: 113.982 ng
RT: 5.457 min Scan# 573
Delta R.T. 0.012 min
Lab File: BF133466.D
Acq: 24 May 2023 12:47

Tgt Ion:112 Resp: 723944
Ion Ratio Lower Upper
112 100
64 60.8 50.2 75.4
63 33.6 27.2 40.8


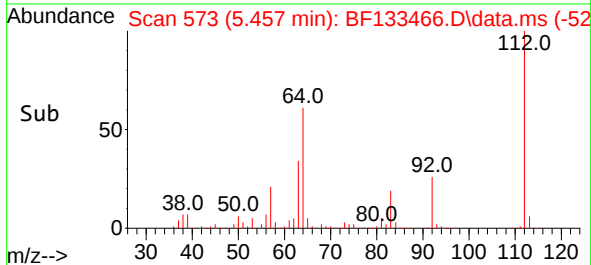
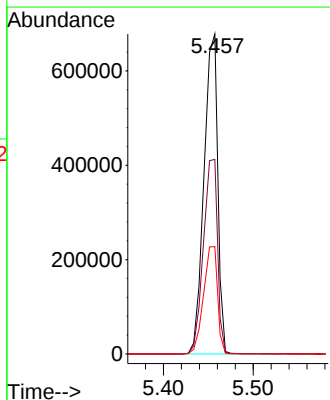
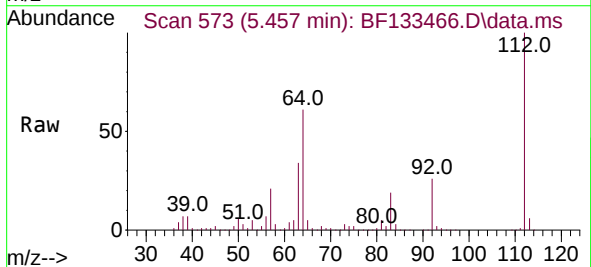


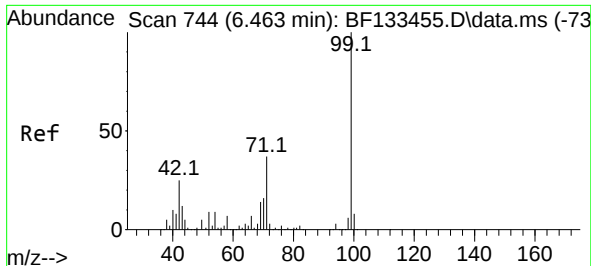

#7
Phenol-d6
Concen: 104.856 ng
RT: 6.463 min Scan# 744
Delta R.T. 0.000 min
Lab File: BF133466.D
Acq: 24 May 2023 12:47




Instrument :
BNA_F
ClientSampleId :
290-328


Tgt Ion: 99 Resp: 800600
Ion Ratio Lower Upper
99 100
42 24.0 19.6 29.4
71 36.1 29.5 44.3

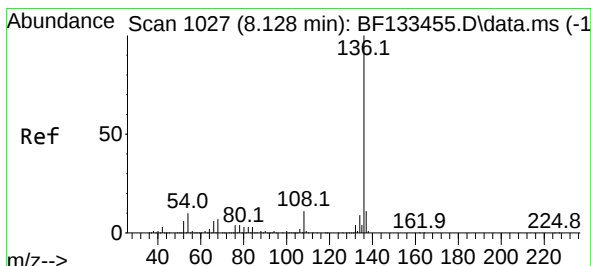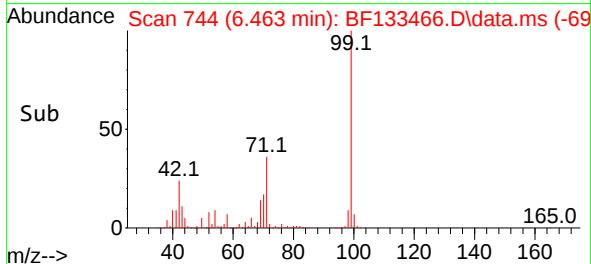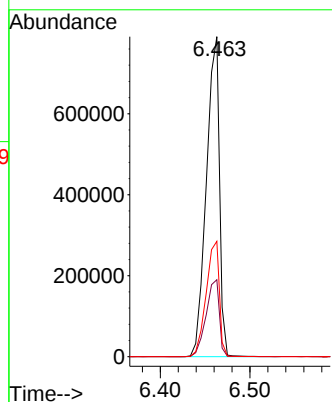

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.122 min Scan# 1026
Delta R.T. -0.006 min
Lab File: BF133466.D
Acq: 24 May 2023 12:47

Tgt Ion:136 Resp: 397740
Ion Ratio Lower Upper
136 100
137 11.1 8.8 13.2
54 9.8 8.0 12.0
68 6.5 5.4 8.2

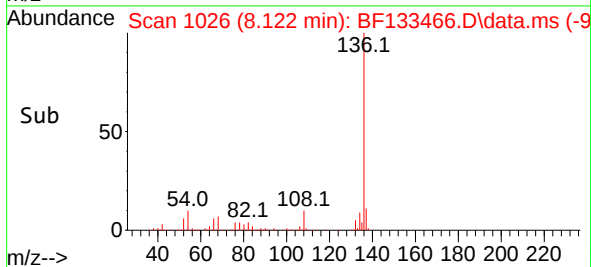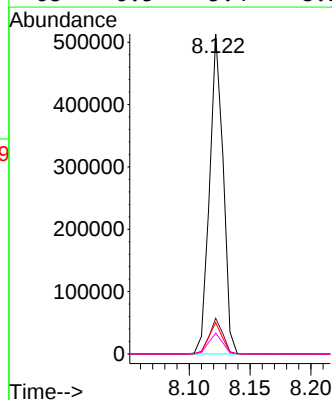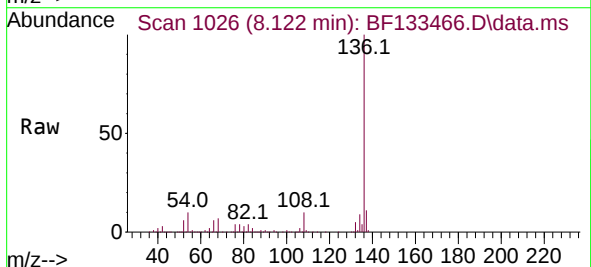

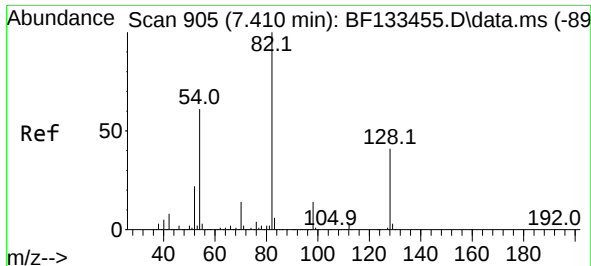

#23

Nitrobenzene-d5

Concen: 105.702 ng

RT: 7.404 min Scan# 905

Delta R.T. -0.006 min

Lab File: BF133466.D

Acq: 24 May 2023 12:47

Instrument :

BNA_F

ClientSampleId :

290-328





Tgt Ion: 82 Resp: 608112

Ion Ratio Lower Upper

82 100

128 43.9 33.0 49.6

54 59.1 48.5 72.7

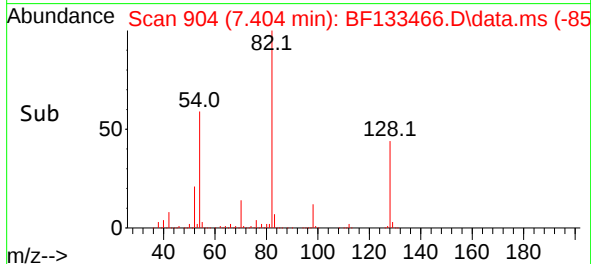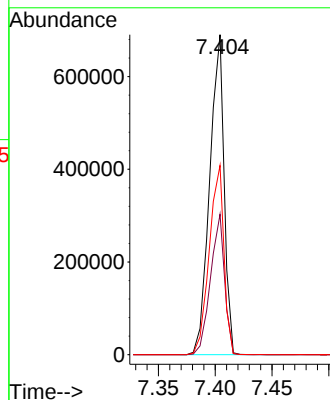

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.875 min Scan# 1324

Delta R.T. -0.005 min

Lab File: BF133466.D

Acq: 24 May 2023 12:47




Tgt Ion: 164 Resp: 193801


Ion Ratio Lower Upper

164 100

162 100.5 79.8 119.6

160 46.2 37.4 56.0

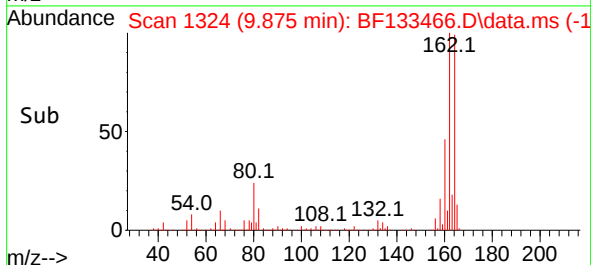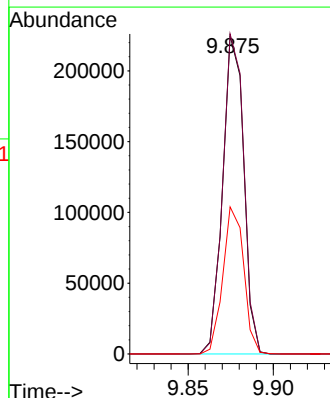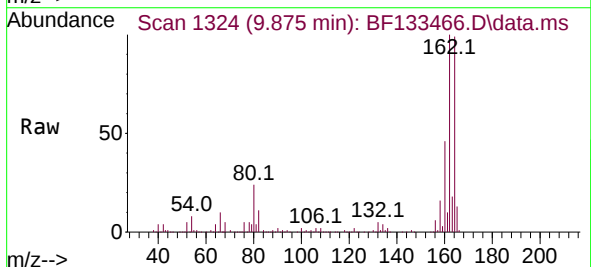

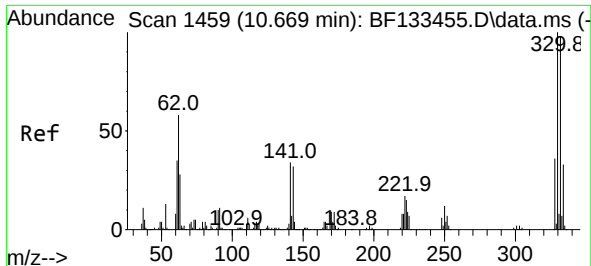

#42

2,4,6-Tribromophenol

Concen: 151.838 ng

RT: 10.669 min Scan# 1459

Delta R.T. 0.000 min

Lab File: BF133466.D


Acq: 24 May 2023 12:47

Instrument :

BNA_F

ClientSampleId :

290-328






Tgt Ion:330 Resp: 271828

Ion Ratio Lower Upper

330 100

332 96.8 77.0 115.6

141 33.8 28.5 42.7

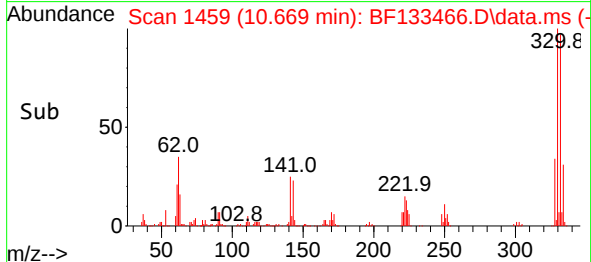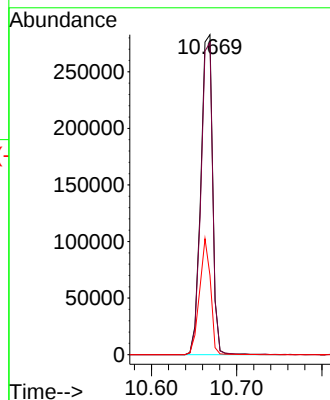

#45

2-Fluorobiphenyl

Concen: 78.950 ng

RT: 9.204 min Scan# 1210

Delta R.T. 0.000 min

Lab File: BF133466.D

Acq: 24 May 2023 12:47




Tgt Ion:172 Resp: 1087516


Ion Ratio Lower Upper

172 100

171 35.8 28.5 42.7

170 24.3 19.0 28.4


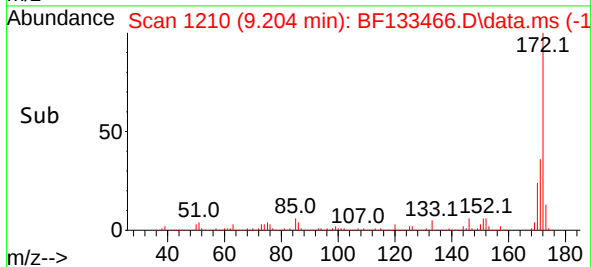
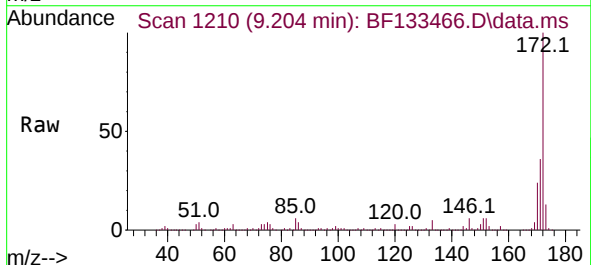
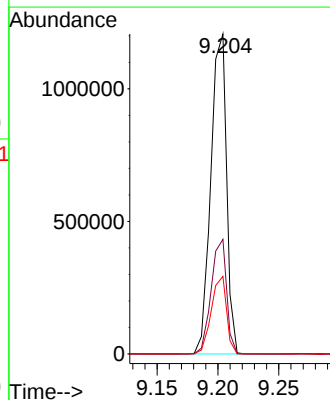


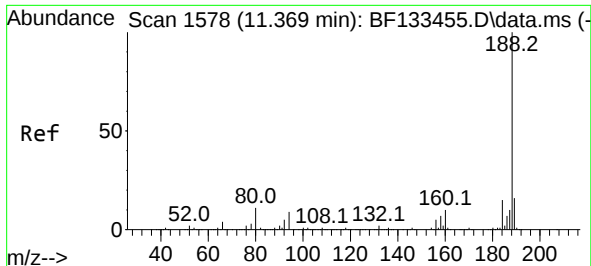

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.363 min Scan# 11
Delta R.T. -0.006 min
Lab File: BF133466.D
Acq: 24 May 2023 12:47




Instrument :
BNA_F
ClientSampleId :
290-328


Tgt Ion:188 Resp: 383973
Ion Ratio Lower Upper
188 100
94 9.9 7.5 11.3
80 11.0 8.7 13.1

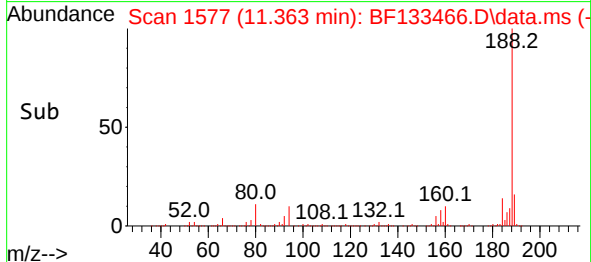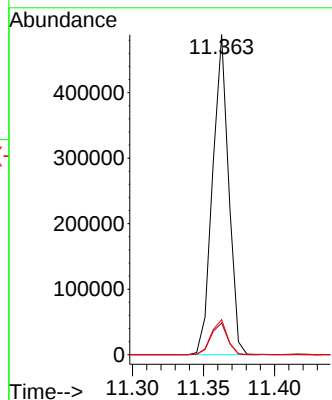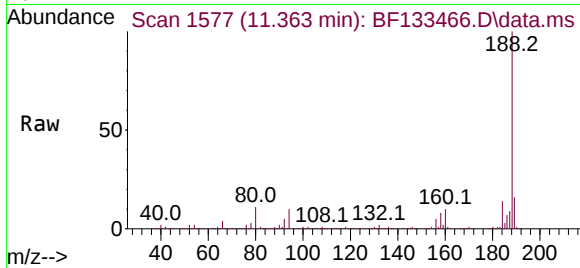

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.004 min Scan# 2026
Delta R.T. -0.006 min
Lab File: BF133466.D
Acq: 24 May 2023 12:47

Tgt Ion:240 Resp: 306300
Ion Ratio Lower Upper
240 100
120 11.6 10.2 15.4
236 26.2 20.9 31.3


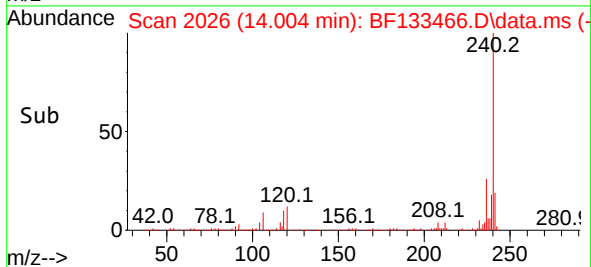
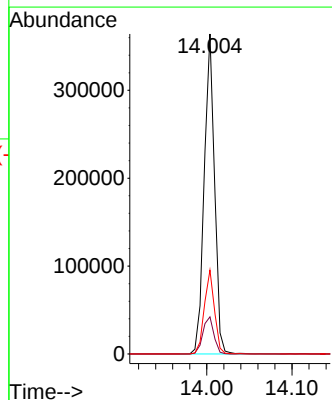
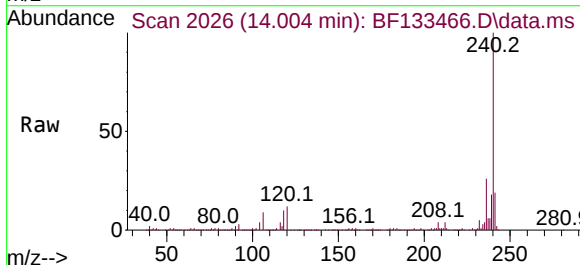


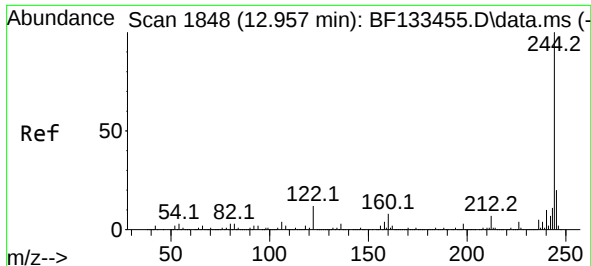

#79
 Terphenyl-d14
 Concen: 84.224 ng
 RT: 12.957 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: BF133466.D
 Acq: 24 May 2023 12:47

Instrument :
 BNA_F
 ClientSampleId :
 290-328

Tgt Ion:244 Resp: 1349321
 Ion Ratio Lower Upper
 244 100
 212 7.1 5.6 8.4
 122 10.7 9.4 14.0

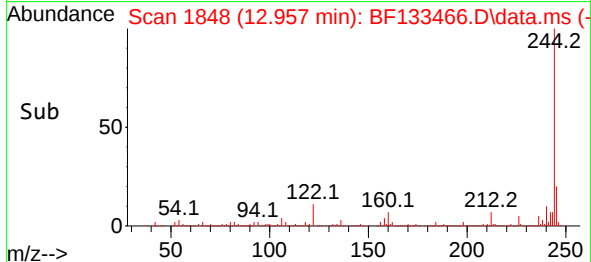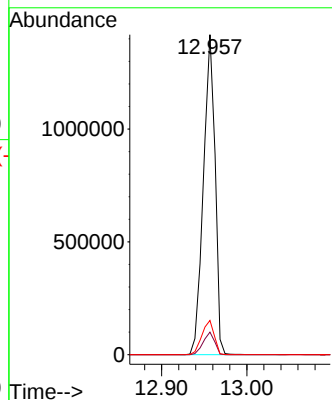

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.462 min Scan# 2274
 Delta R.T. -0.006 min
 Lab File: BF133466.D
 Acq: 24 May 2023 12:47

Tgt Ion:264 Resp: 277045
 Ion Ratio Lower Upper
 264 100
 260 24.8 18.8 28.2
 265 21.0 17.0 25.4

