
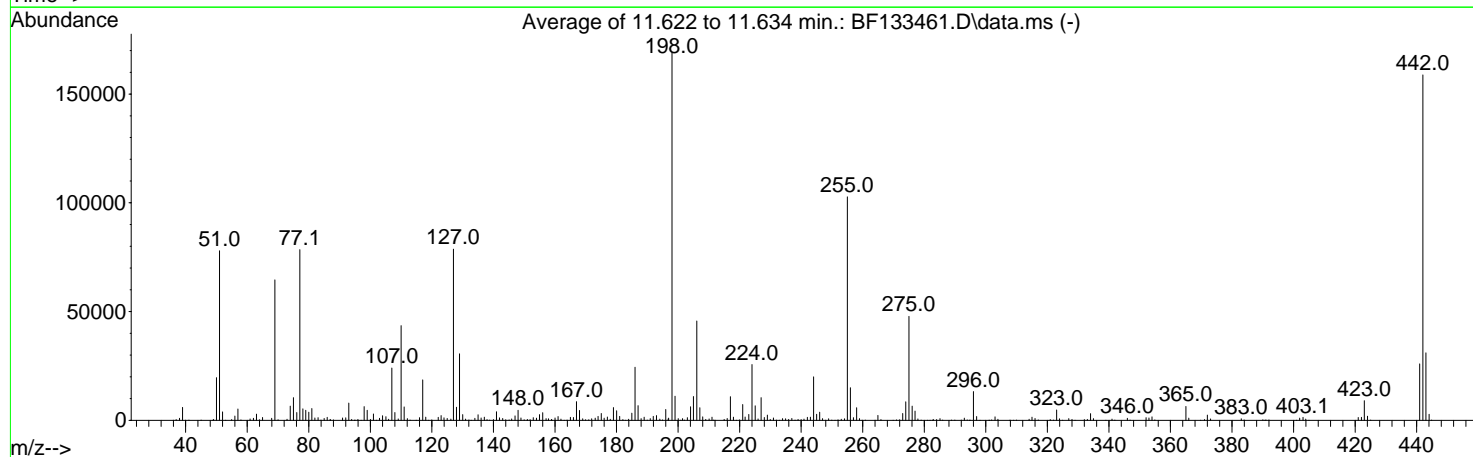


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052423\
 Data File : BF133461.D
 Acq On : 24 May 2023 10:10
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052323.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 24 02:41:39 2023

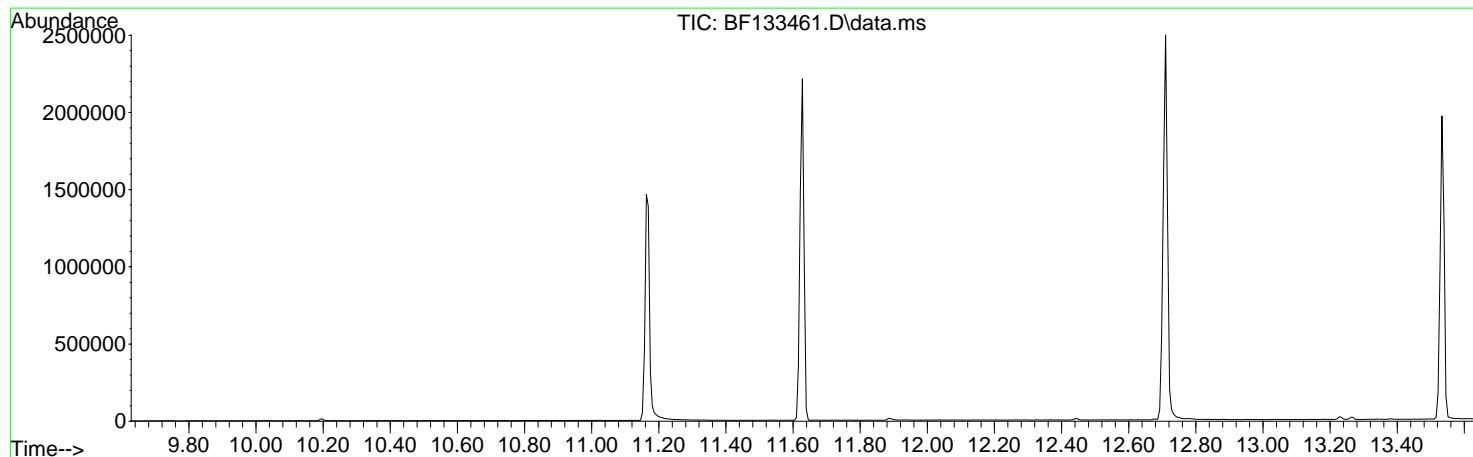

AutoFind: Scans 1621, 1622, 1623; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.1	77933	PASS
68	69	0.00	2	1.5	990	PASS
69	198	0.00	100	38.2	64557	PASS
70	69	0.00	2	0.5	301	PASS
127	198	10	80	46.5	78680	PASS
197	198	0.00	2	0.6	1071	PASS
198	198	100	100	100.0	169096	PASS
199	198	5	9	6.6	11109	PASS
275	198	10	60	28.3	47821	PASS
365	198	1	100	3.8	6427	PASS
441	198	0.01	100	15.4	25957	PASS
442	442	50	100	100.0	158784	PASS
443	442	15	24	19.6	31053	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/24/2023	BNA_F	<u>BF133461.D</u>
Compound Name	Response	Retention Time
DDT	285494	13.533
DDD	5320	13.233
DDE	0	12.896
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5320	290814	1.83

Instrument :
 BNA_F
 ClientSampled :
 DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052423\
 Data File : BF133461.D
 Acq On : 24 May 2023 10:10
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 24 13:47:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 24 02:41:39 2023
 Response via : Initial Calibration

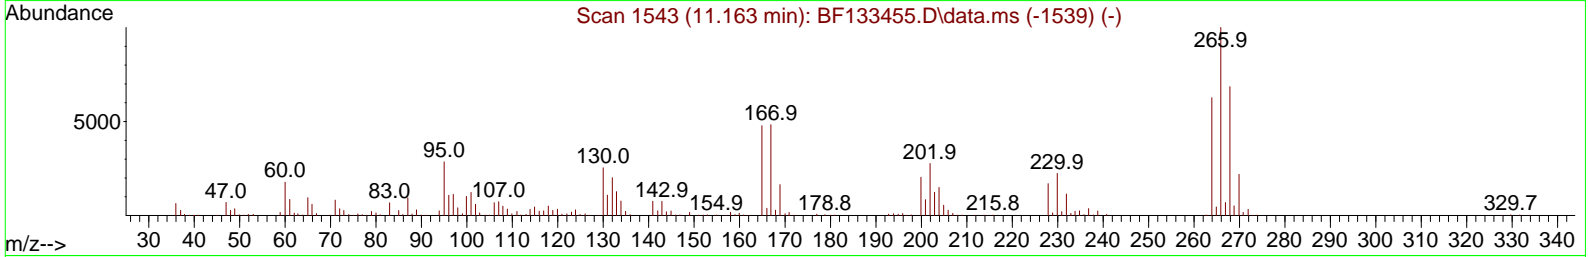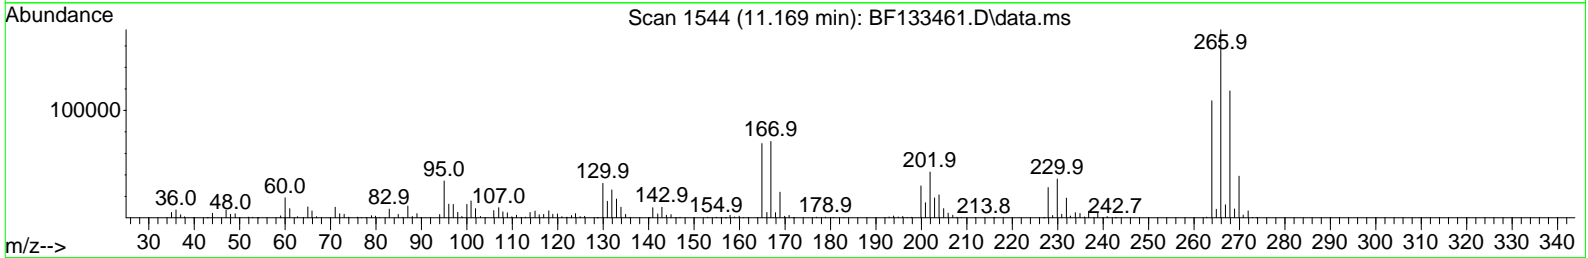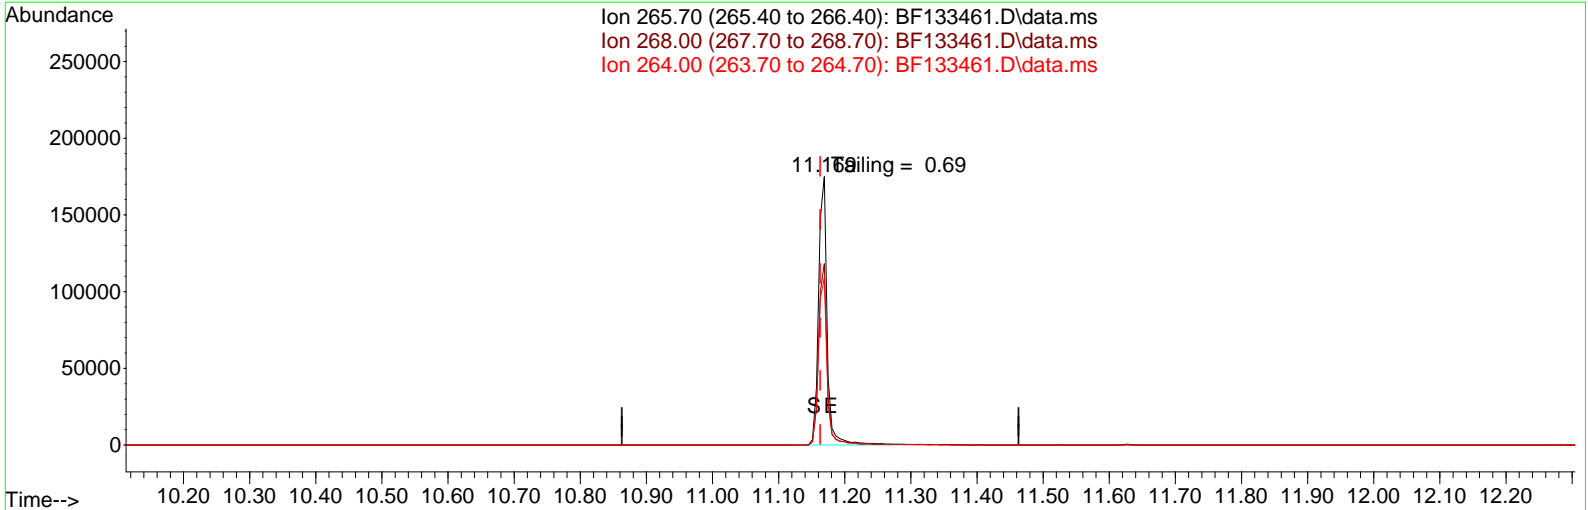

TIC: BF133461.D\data.ms

(70) Pentachlorophenol (C)

11.169min (+ 0.006) 470188.66 ng




response 158584

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	68.50	67.53
264.00	62.70	62.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052423\
 Data File : BF133461.D
 Acq On : 24 May 2023 10:10
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 24 13:47:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 24 02:41:39 2023
 Response via : Initial Calibration

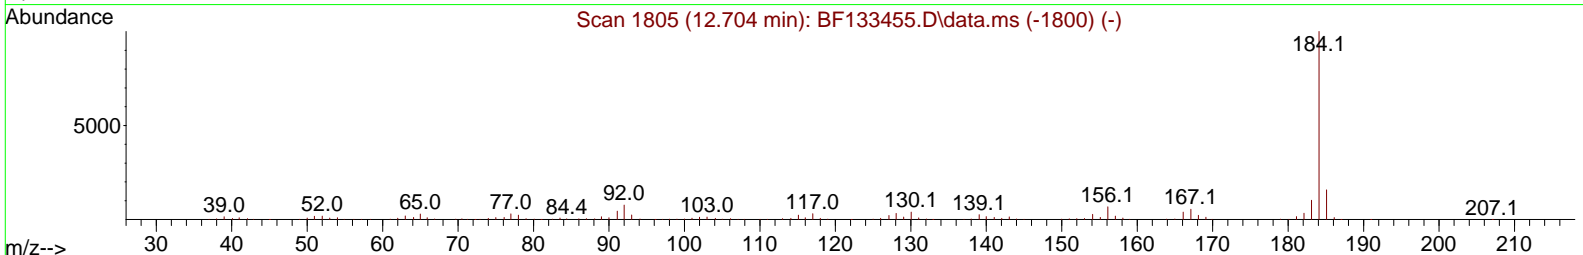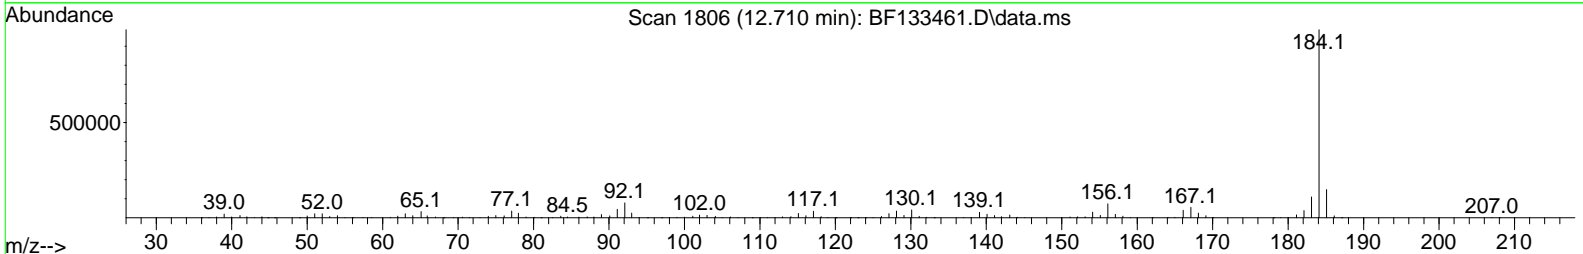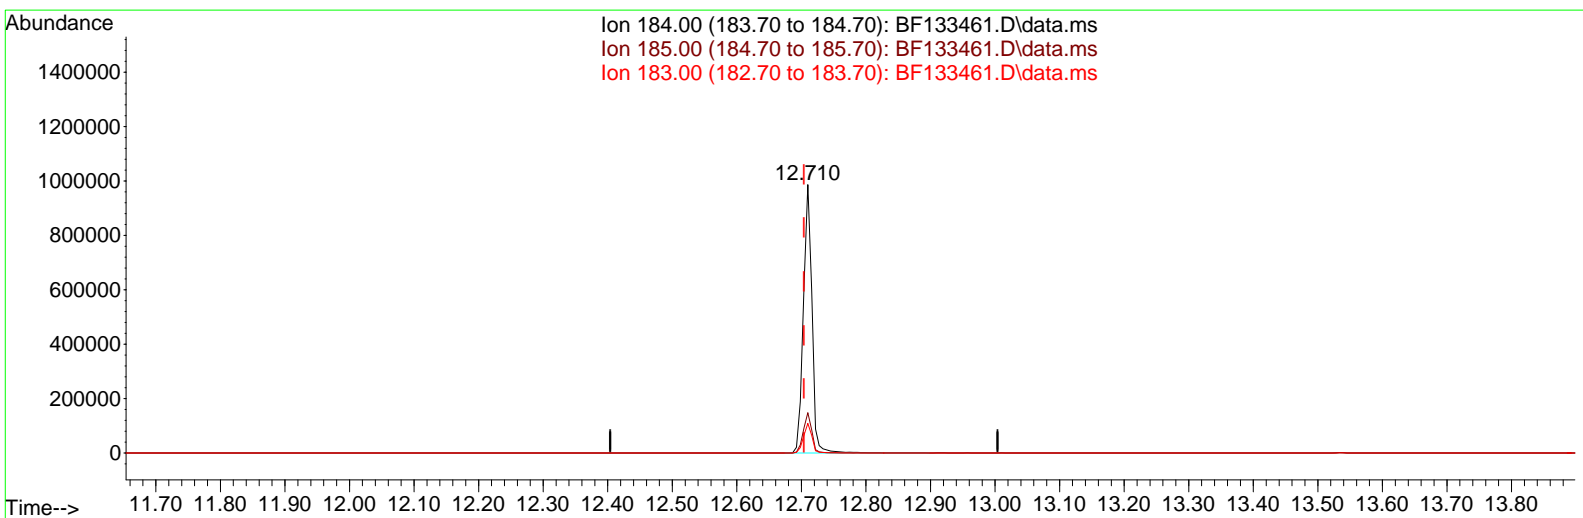

TIC: BF133461.D\data.ms

(77) Benzidine

12.710min (+ 0.006)	0.00 ng
response	924409
Ion	Exp% Act%
184.00	100.00 100.00
185.00	15.80 15.02
183.00	10.20 11.07
0.00	0.00 0.00