
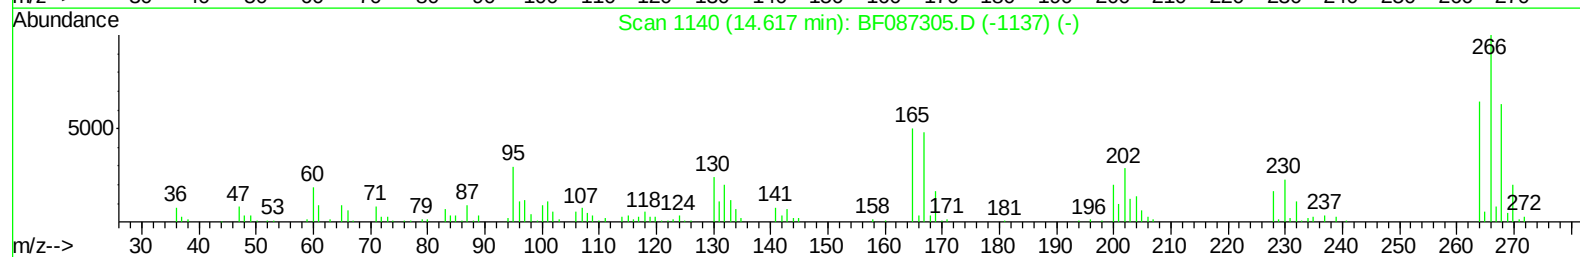
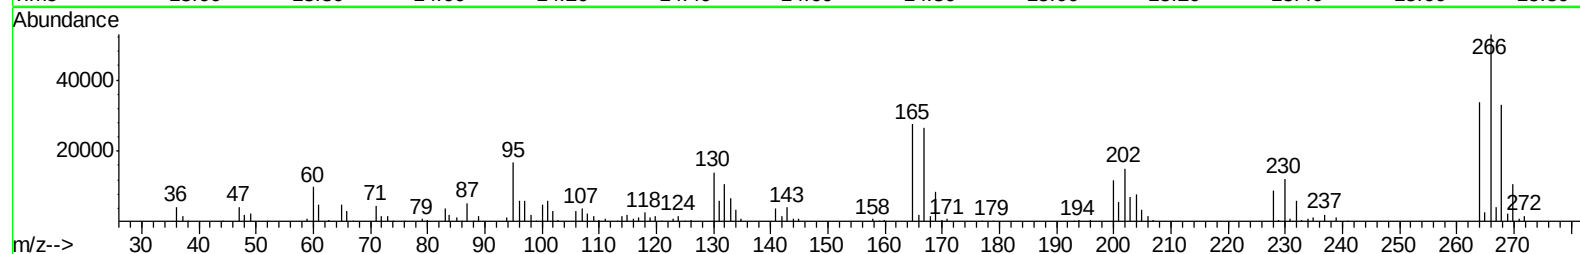


Data Path : Z:\HPCHEM1\BNA F\Data\BF052516\
Data File : BF087366.D
Acq On : 25 May 2016 10:39
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 25 11:35:55 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 24 01:40:43 2016
Response via : Initial Calibration

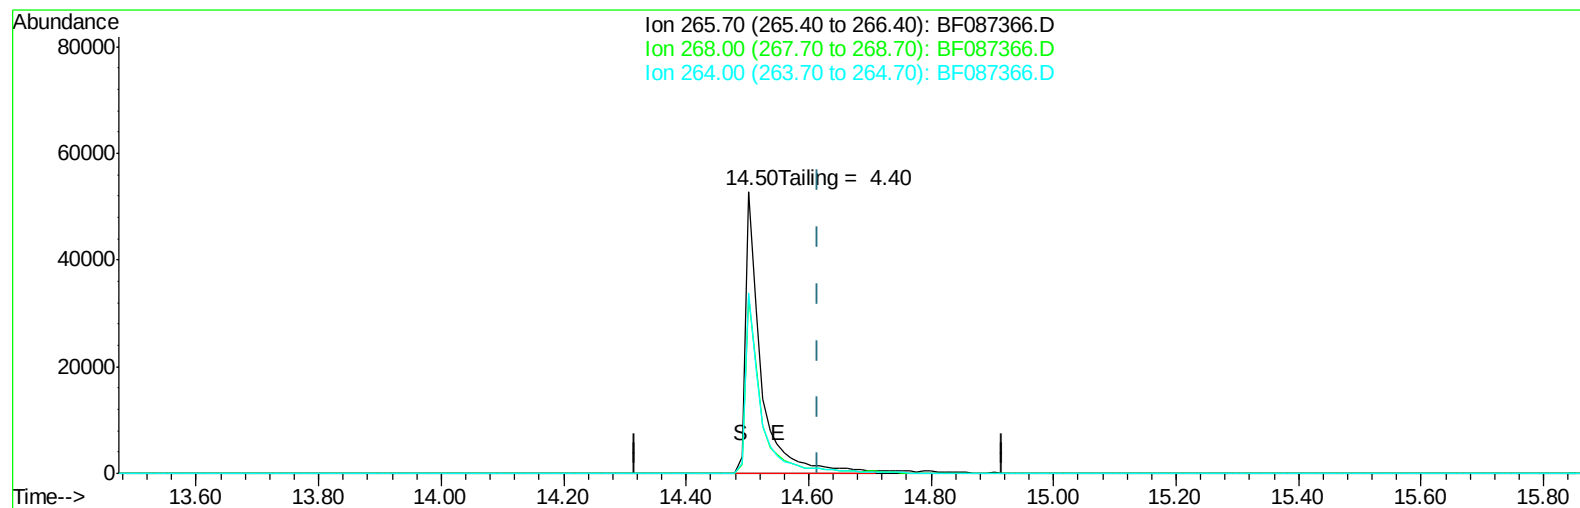

TIC: BF087366.D

(69) Pentachlorophenol (C)




14.502min (-0.114) 0.00ng

response 95675

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	62.63
264.00	66.10	64.07
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF052516\
Data File : BF087366.D
Acq On : 25 May 2016 10:39
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 25 11:35:55 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 24 01:40:43 2016
Response via : Initial Calibration

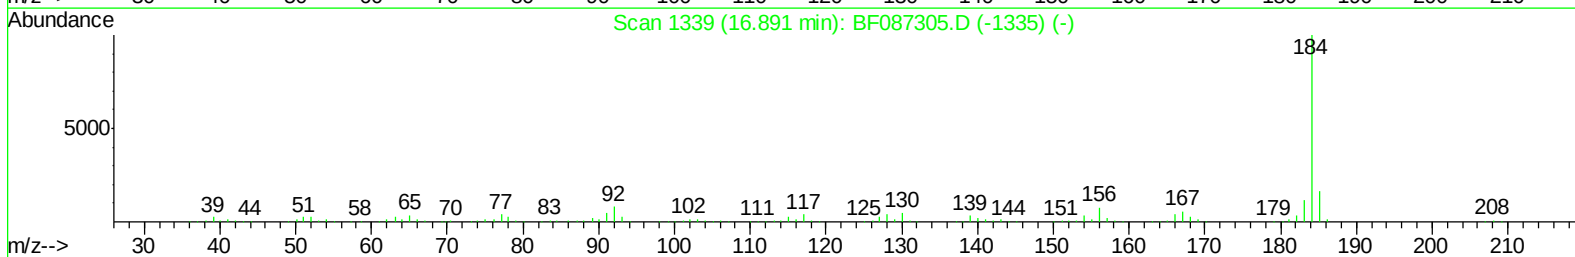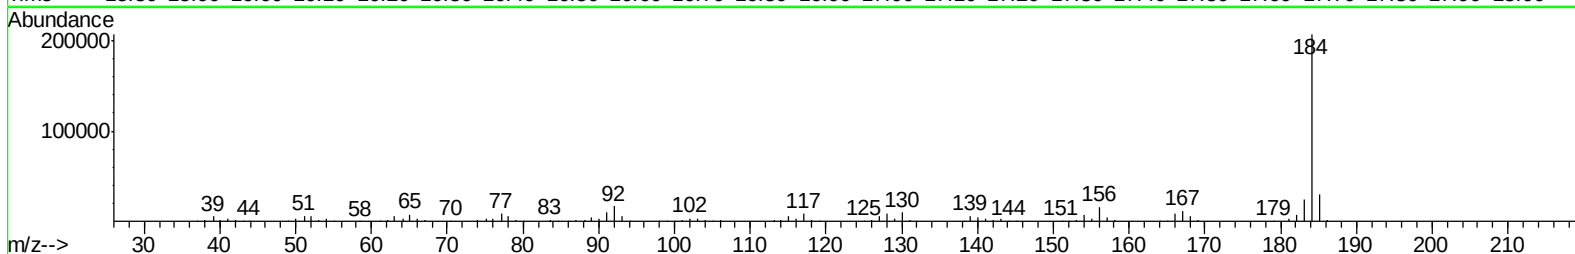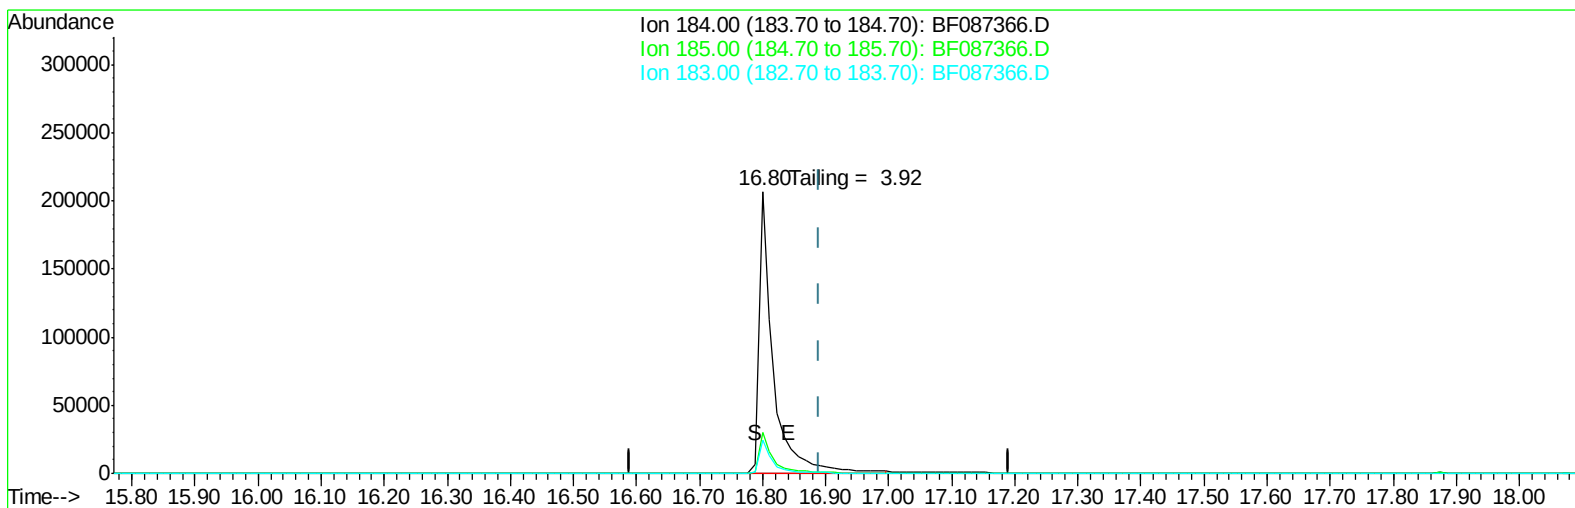

TIC: BF087366.D

(76) Benzidine

16.800min (-0.091) 0.00ng

response 328425

Ion	Exp%	Act%
184.00	100	100
185.00	17.00	14.68
183.00	12.20	11.66
0.00	0.00	0.00