
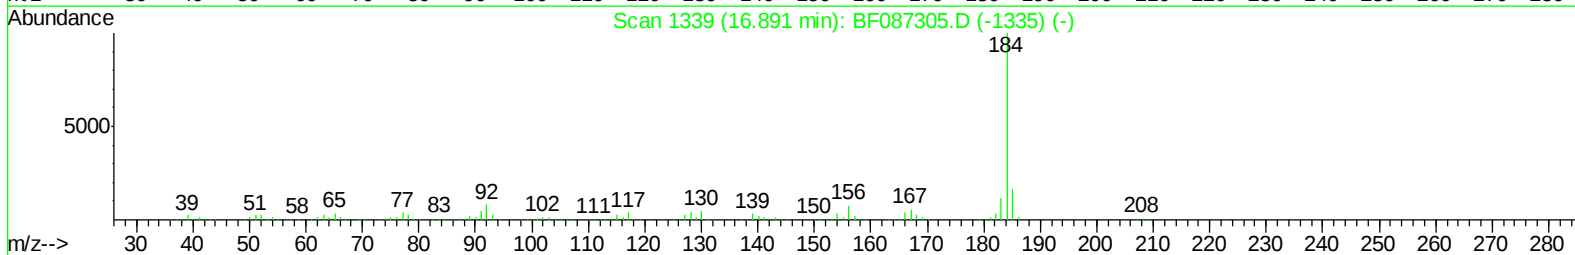
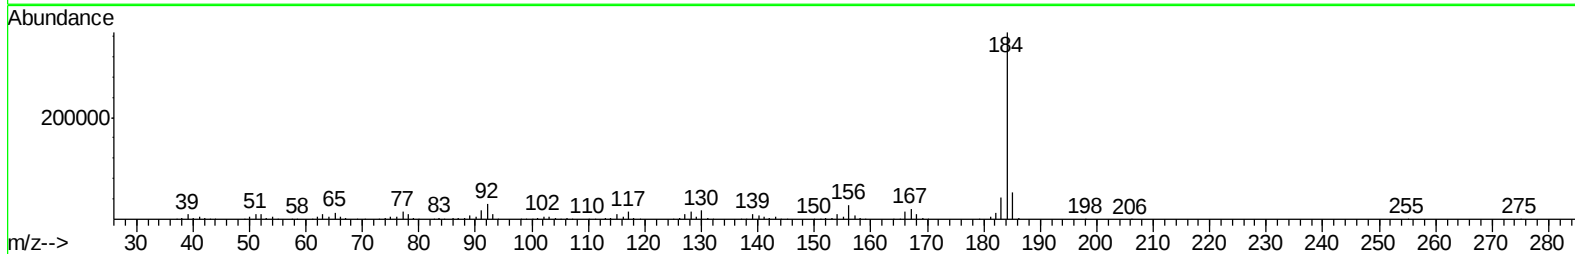


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052516\
Data File : BF087385.D
Acq On : 25 May 2016 23:03
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 26 04:43:57 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 25 16:26:52 2016
Response via : Initial Calibration

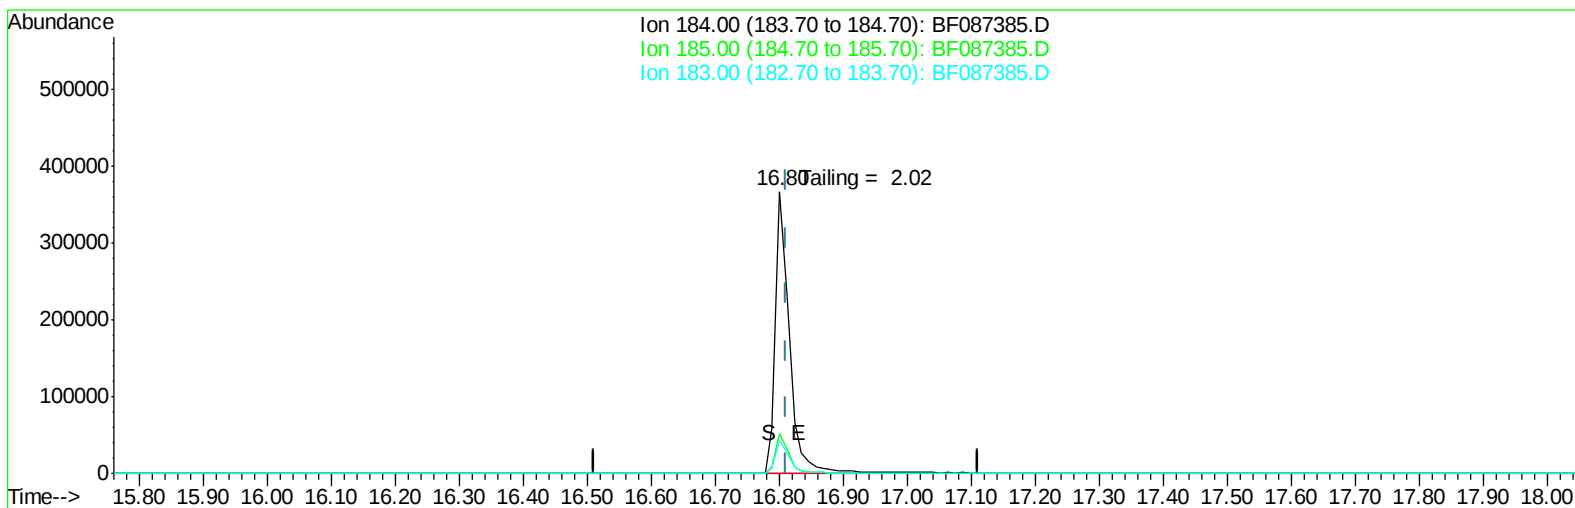

TIC: BF087385.D

(76) Benzidine




16.800min (-0.011) 0.00ng

response 557980

Ion	Exp%	Act%
184.00	100	100
185.00	17.00	14.27
183.00	12.20	11.62
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052516\
Data File : BF087385.D
Acq On : 25 May 2016 23:03
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 26 04:43:57 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 25 16:26:52 2016
Response via : Initial Calibration

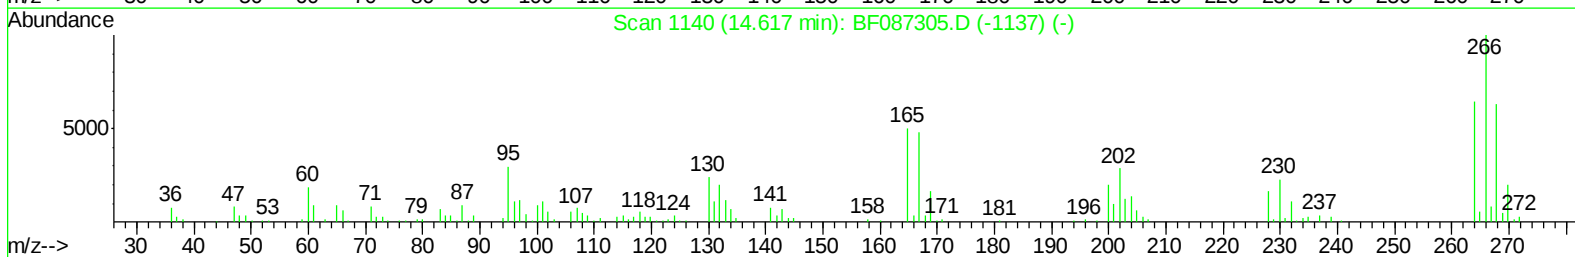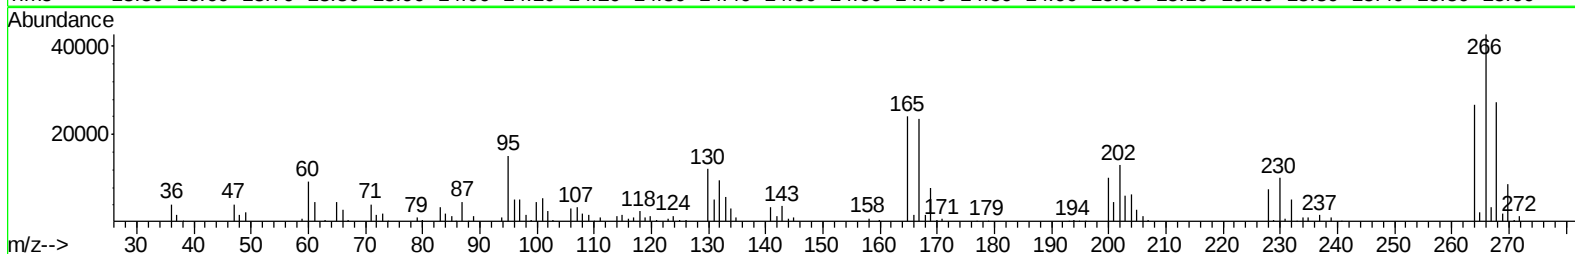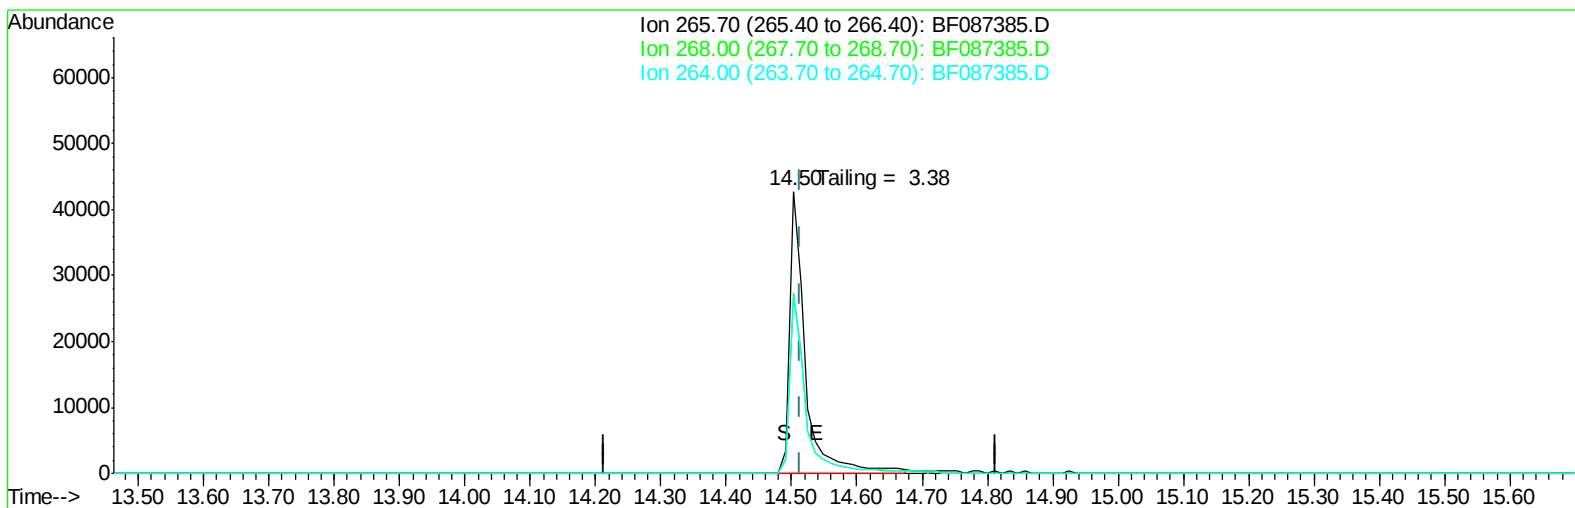

TIC: BF087385.D

(69) Pentachlorophenol (C)

14.502min (-0.011) 0.00ng

response 72648

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	63.97
264.00	66.10	62.79
0.00	0.00	0.00