

Data Path : Z:\HPCHEM1\BNA F\DATA\BF052516\
 Data File : BF087396.D
 Acq On : 26 May 2016 5:20
 Operator : UM/SJ
 Sample : H3220-04
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-34-COMP

Quant Time: May 26 08:42:23 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF052316.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 25 16:26:52 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.52	152	97532	20.00	ng	0.00
21) Naphthalene-d8	9.55	136	375587	20.00	ng	0.00
38) Acenaphthene-d10	12.38	164	153653	20.00	ng	-0.01
63) Phenanthrene-d10	14.78	188	247161	20.00	ng	0.00
75) Chrysene-d12	18.47	240	215217	20.00	ng	-0.01
86) Perylene-d12	20.14	264	143133	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.45	112	887477	159.89	ng	0.03
7) Phenol-d6	7.10	99	1125560	150.07	ng	0.02
23) Nitrobenzene-d5	8.44	82	809465	108.62	ng	0.00
41) 2,4,6-Tribromophenol	13.68	330	195817	132.62	ng	0.00
44) 2-Fluorobiphenyl	11.34	172	1200007	110.10	ng	0.00
78) Terphenyl-d14	17.13	244	866980	85.64	ng	0.00
Target Compounds						
49) Dimethylphthalate	12.02	163	352932	28.67	ng	Qvalue 100
83) Bis(2-ethylhexyl)phthalate	18.54	149	27041	2.70	ng	# 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF052516\
Data File : BF087396.D
Acq On : 26 May 2016 5:20
Operator : UM/SJ
Sample : H3220-04
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-34-COMP

Quant Time: May 26 08:42:23 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 25 16:26:52 2016
Response via : Initial Calibration

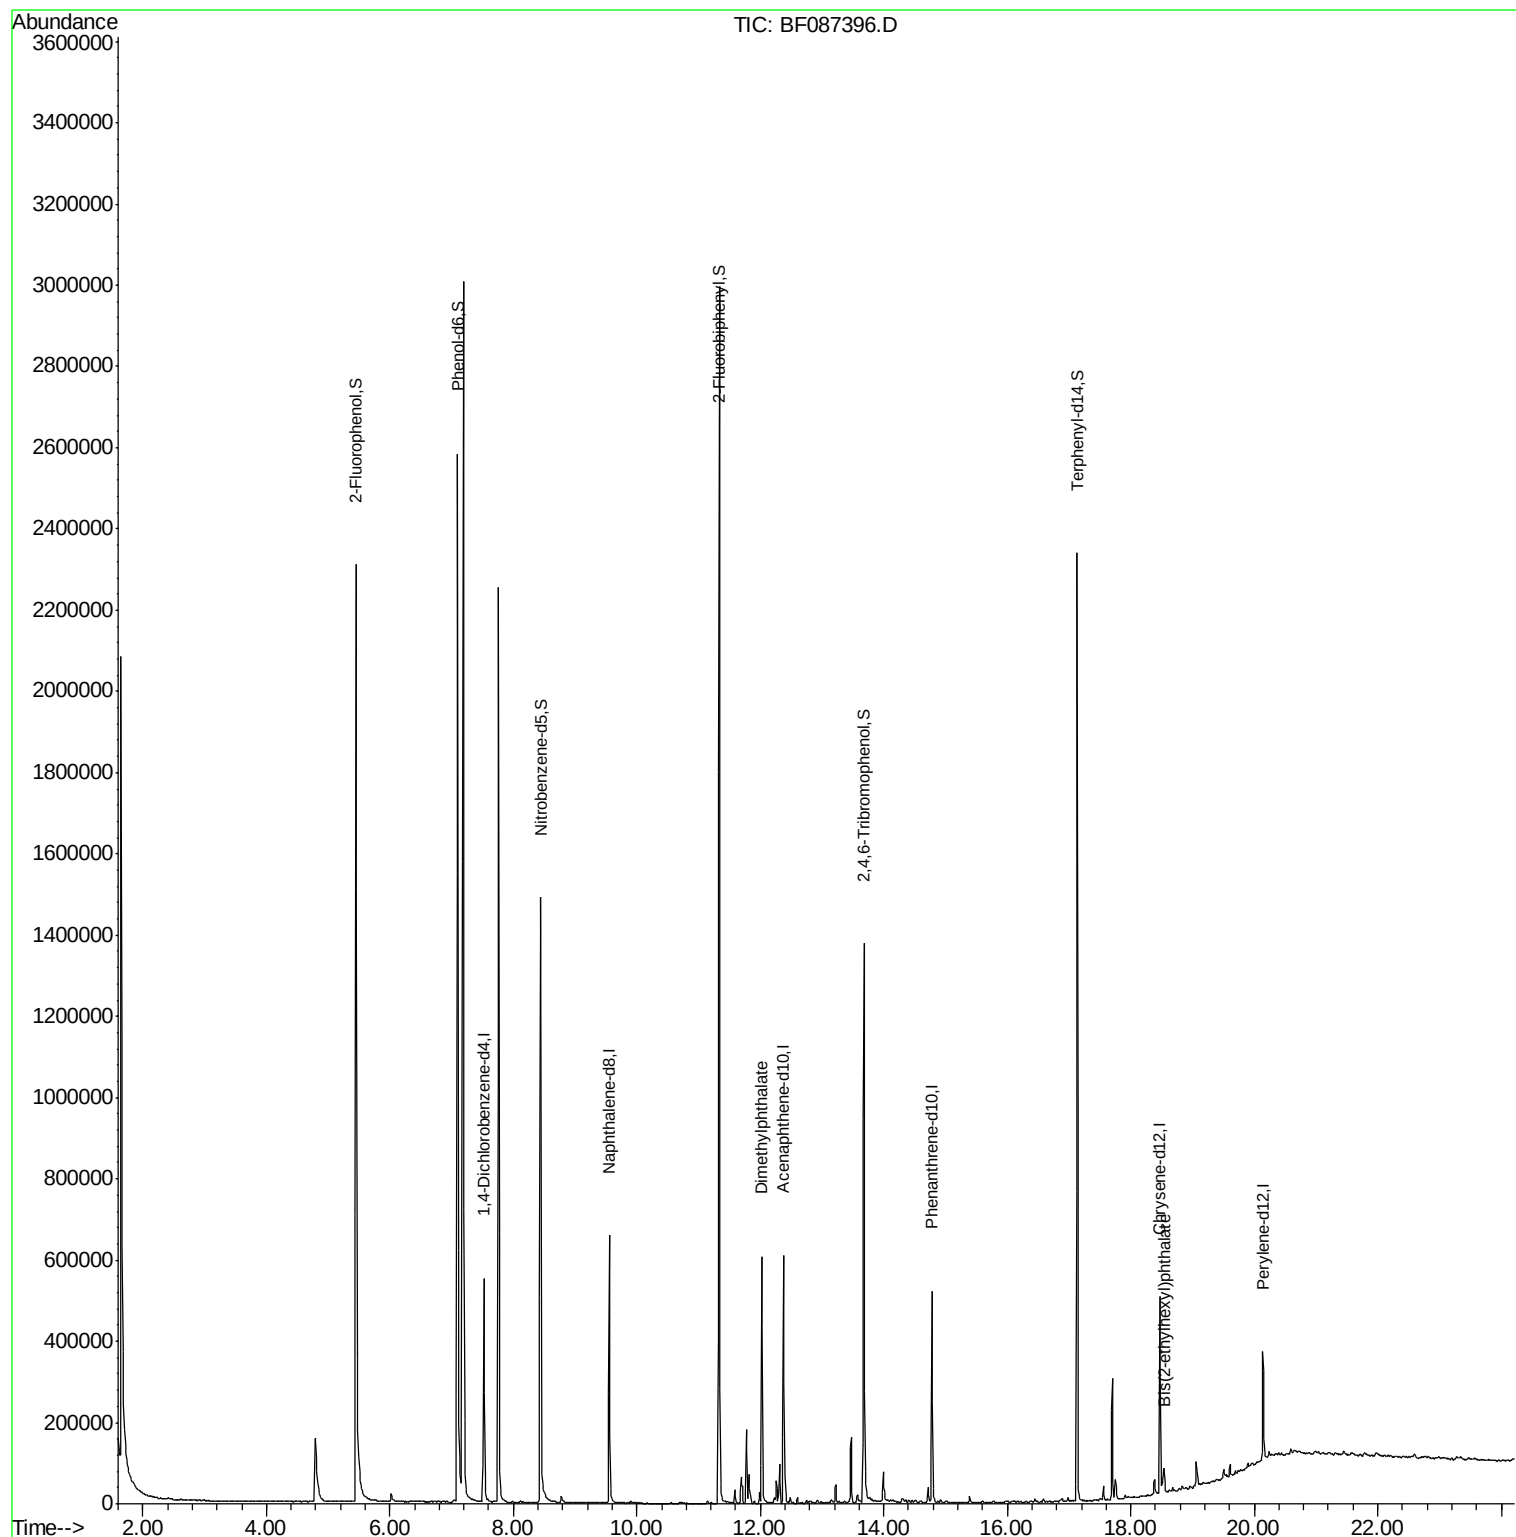

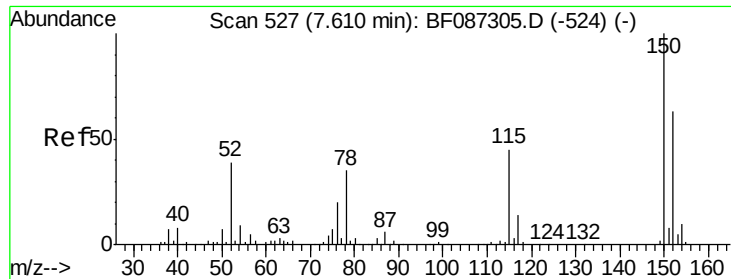

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 7.52 min Scan# 519

Delta R.T. -0.00 min

Lab File: BF087396.D

Acq: 26 May 2016 5:20

Instrument :

BNA_F

ClientSampleId :

SB-34-COMP





Tot Ion:152 Resp: 97532

Ion Ratio Lower Upper

152 100

150 156.1 125.8 188.6

115 72.9 51.5 77.3

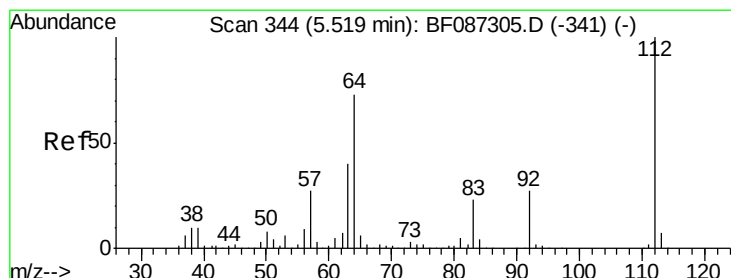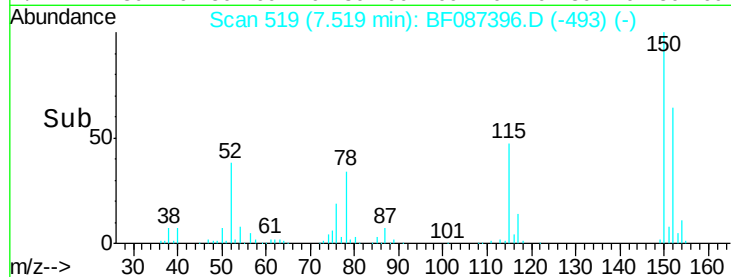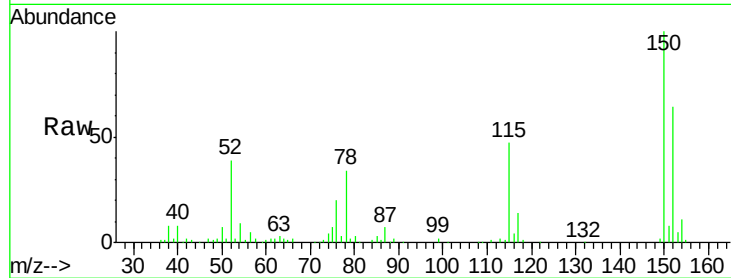

#5

2-Fluorophenol

Concen: 159.89 ng

RT: 5.45 min Scan# 338

Delta R.T. 0.03 min

Lab File: BF087396.D

Acq: 26 May 2016 5:20




Tgt Ion:112 Resp: 887477


Ion Ratio Lower Upper

112 100

64 78.6 52.1 78.1#

63 44.2 25.7 38.5#

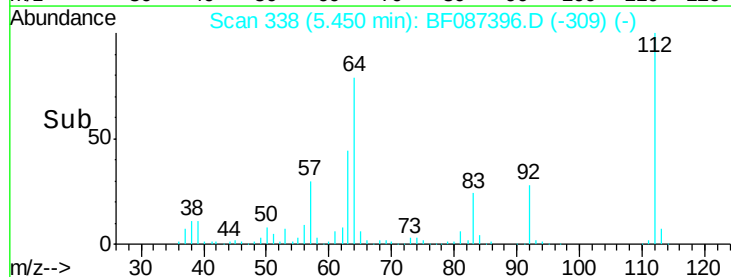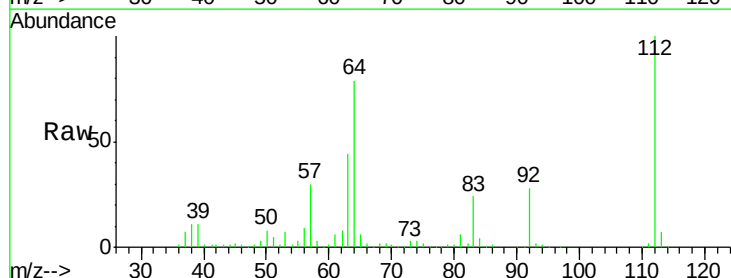

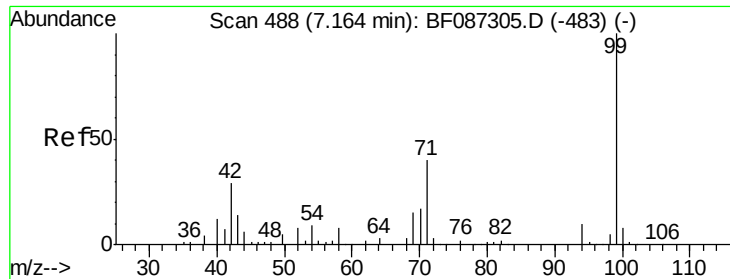

#7

Phenol-d6

Concen: 150.07 ng

RT: 7.10 min Scan# 482

Delta R.T. 0.02 min

Lab File: BF087396.D

Acq: 26 May 2016 5:20

Instrument :

BNA_F

ClientSampleId :

SB-34-COMP


Tot Ion: 99 Resp: 1125560

Ion Ratio Lower Upper

99 100

42 31.6 13.6 20.4#




71 42.3 24.6 36.8#

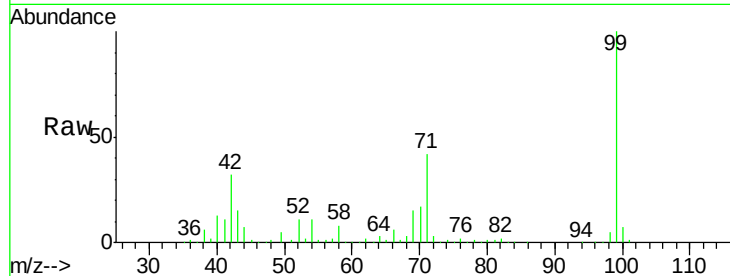

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

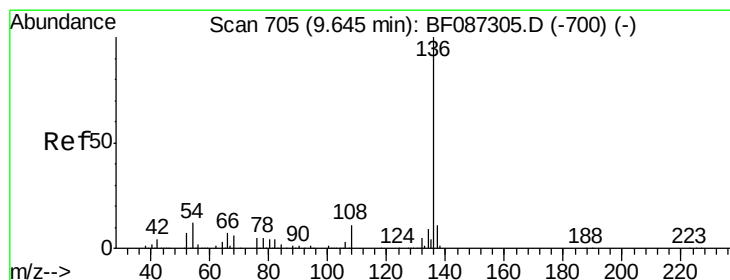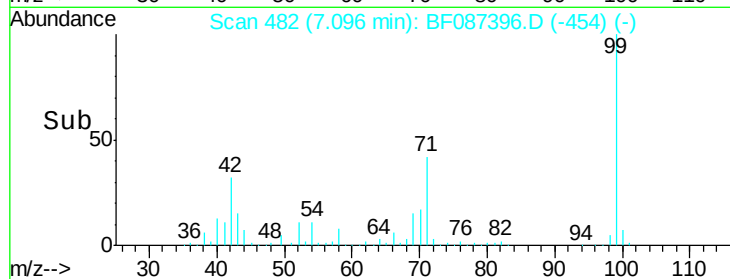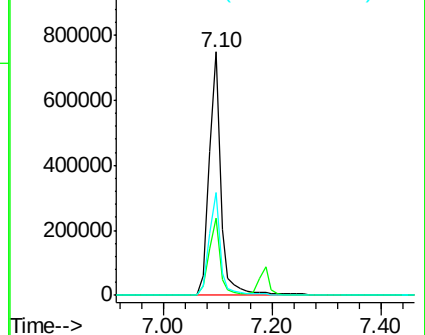

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 9.55 min Scan# 697

Delta R.T. -0.00 min

Lab File: BF087396.D

Acq: 26 May 2016 5:20

Tgt Ion: 136 Resp: 375587


Ion Ratio Lower Upper

136 100

137 10.9 8.8 13.2

54 10.8 5.0 7.4#

68 5.4 4.4 6.6


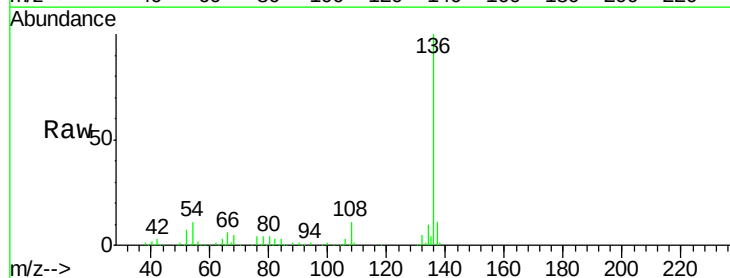



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

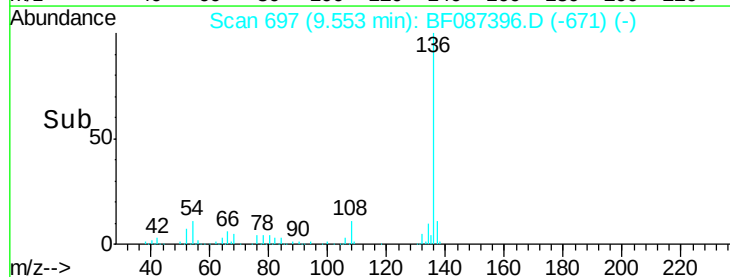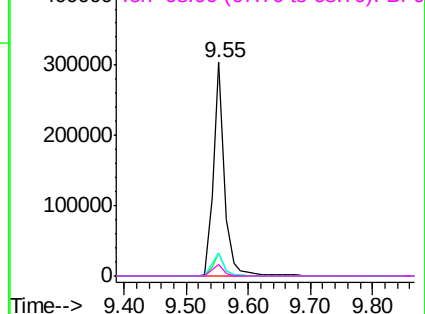

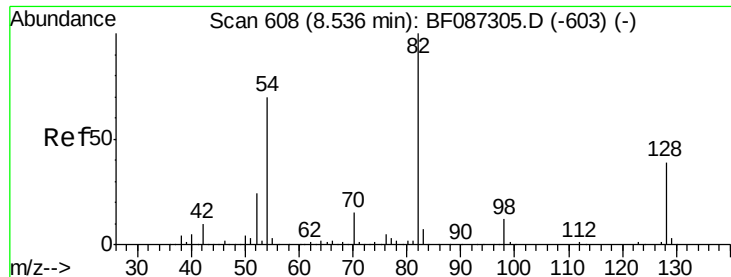

#23

Nitrobenzene-d5

Concen: 108.62 ng

RT: 8.44 min Scan# 600

Delta R.T. -0.00 min

Lab File: BF087396.D

Acq: 26 May 2016 5:20

Instrument :

BNA_F

ClientSampleId :

SB-34-COMP


Tot Ion: 82 Resp: 809465

Ion Ratio Lower Upper




82 100

128 42.4 40.6 61.0

54 65.3 38.1 57.1#

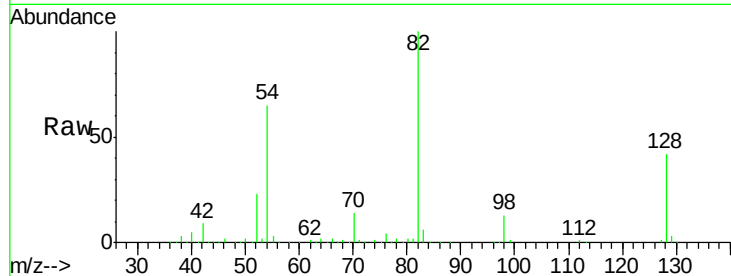

Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0

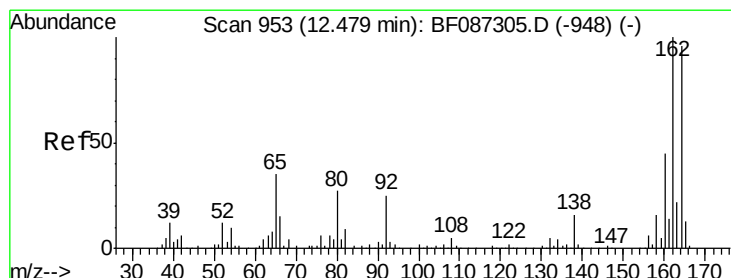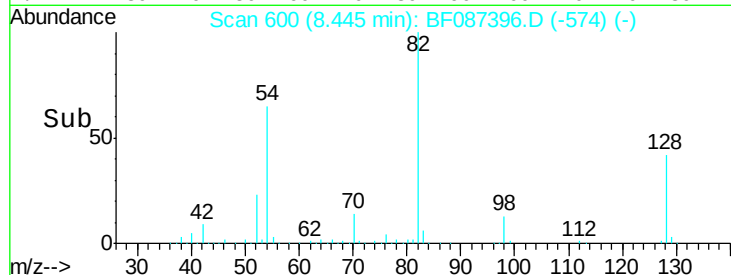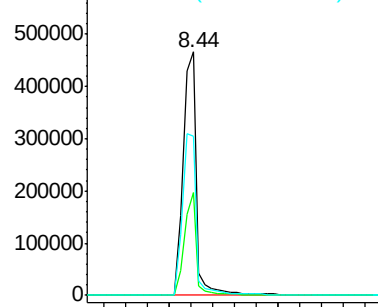

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 12.38 min Scan# 944

Delta R.T. -0.01 min

Lab File: BF087396.D

Acq: 26 May 2016 5:20


Tgt Ion:164 Resp: 153653

Ion Ratio Lower Upper



164 100


162 102.6 82.8 124.2

160 47.3 36.9 55.3

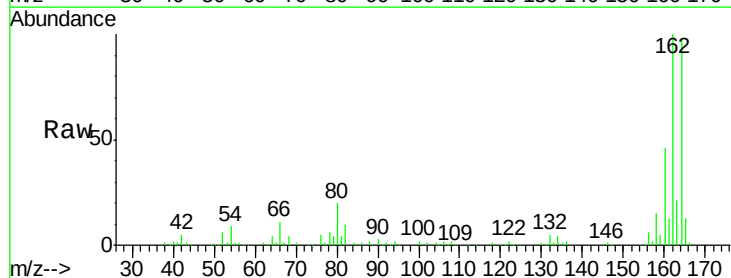

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

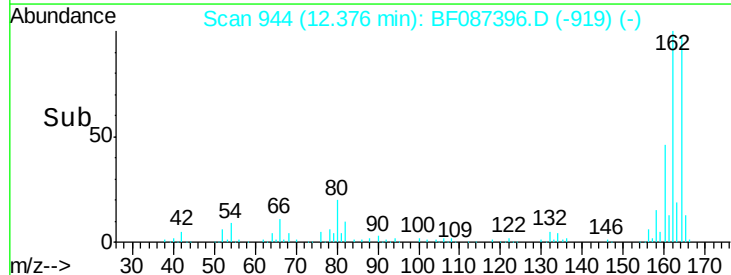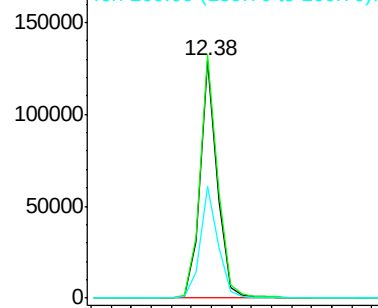


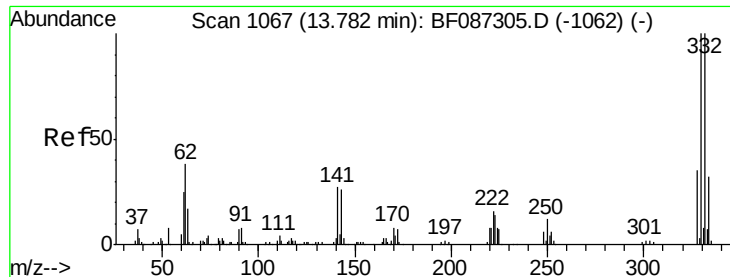

#41
 2,4,6-Tribromophenol
 Concen: 132.62 ng
 RT: 13.68 min Scan# 1058
 Delta R.T. -0.00 min
 Lab File: BF087396.D
 Acq: 26 May 2016 5:20

Instrument :
 BNA_F
 ClientSampleId :
 SB-34-COMP

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.3	79.0	118.4
141	46.3	31.2	46.8



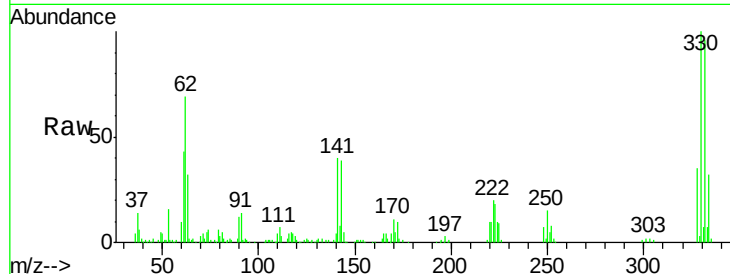


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

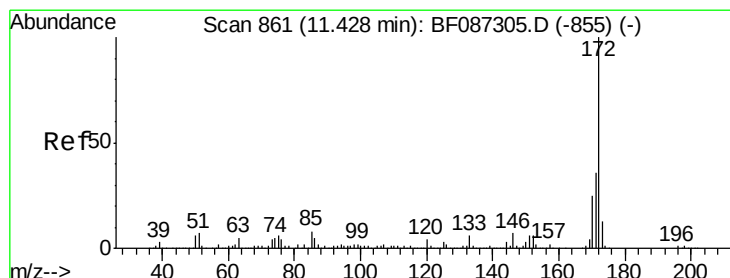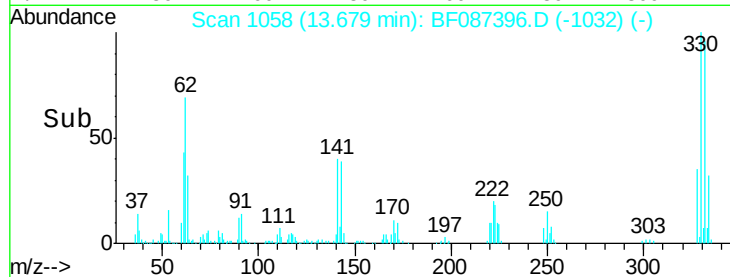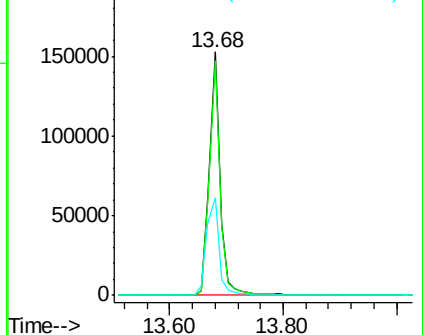

#44
 2-Fluorobiphenyl
 Concen: 110.10 ng
 RT: 11.34 min Scan# 853
 Delta R.T. -0.00 min
 Lab File: BF087396.D
 Acq: 26 May 2016 5:20

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.4	29.0	43.6
170	24.3	19.8	29.8


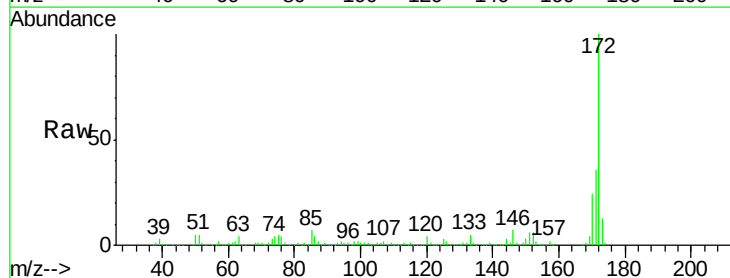



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

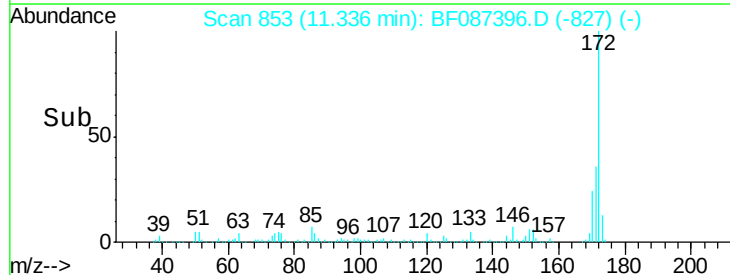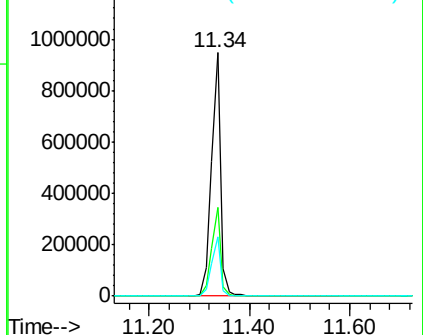

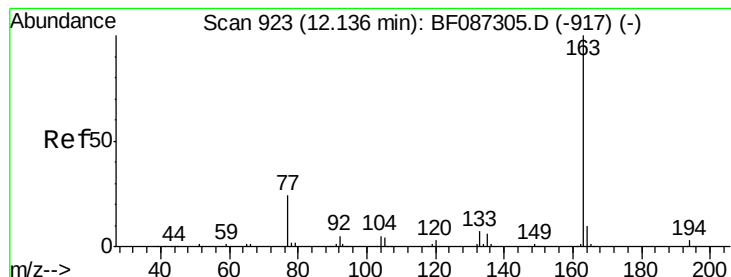

#49

Dimethylphthalate

Concen: 28.67 ng

RT: 12.02 min Scan# 913

Delta R.T. -0.02 min

Lab File: BF087396.D

Acq: 26 May 2016 5:20

Instrument :

BNA_F

ClientSampleId :

SB-34-COMP


Tot Ion:163 Resp: 352932

Ion Ratio Lower Upper

163 100

194 3.1 2.6 4.0




164 10.2 8.2 12.4

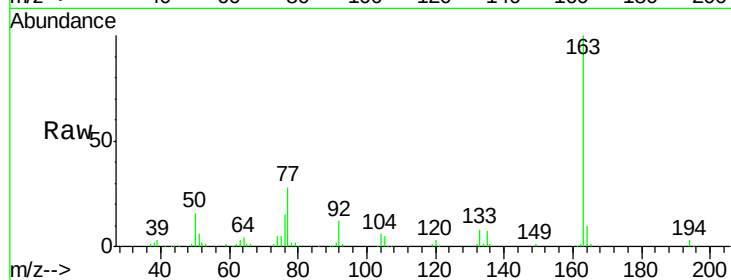

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

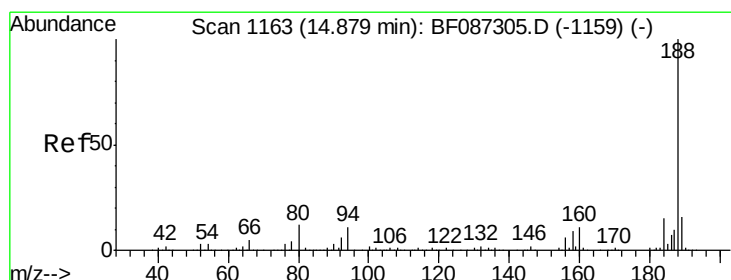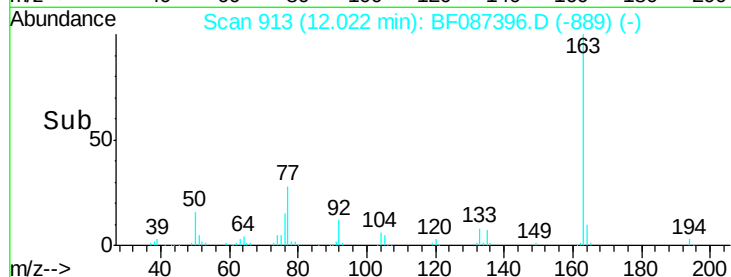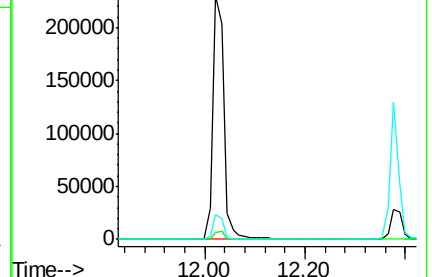

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 14.78 min Scan# 1154

Delta R.T. -0.00 min

Lab File: BF087396.D

Acq: 26 May 2016 5:20


Tgt Ion:188 Resp: 247161

Ion Ratio Lower Upper

188 100

94 9.5 6.8 10.2



80 10.4 7.1 10.7

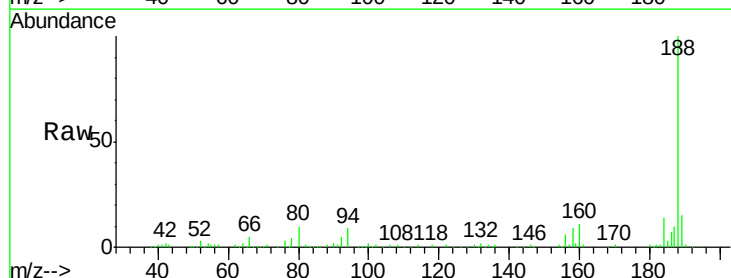


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

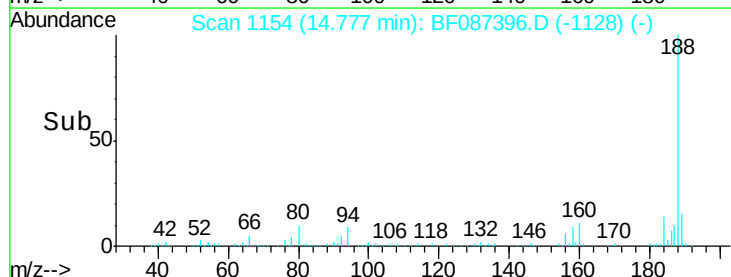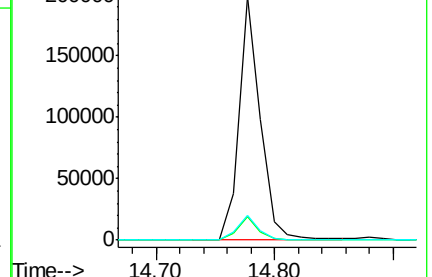

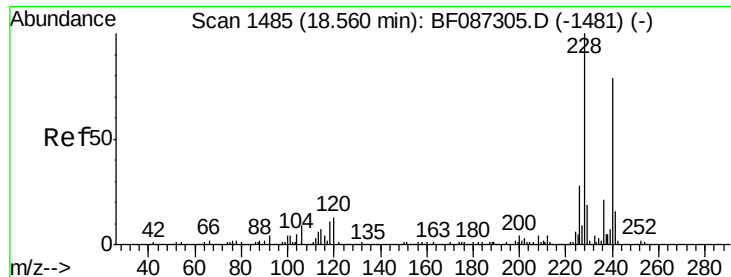

#75

Chrysene-d12

Concen: 20.00 ng

RT: 18.47 min Scan# 1477

Delta R.T. -0.01 min

Lab File: BF087396.D

Acq: 26 May 2016 5:20

Instrument :

BNA_F

ClientSampleId :

SB-34-COMP


Tot Ion:240 Resp: 215217

Ion Ratio Lower Upper

240 100

120 13.3 11.2 16.8




236 25.9 21.2 31.8

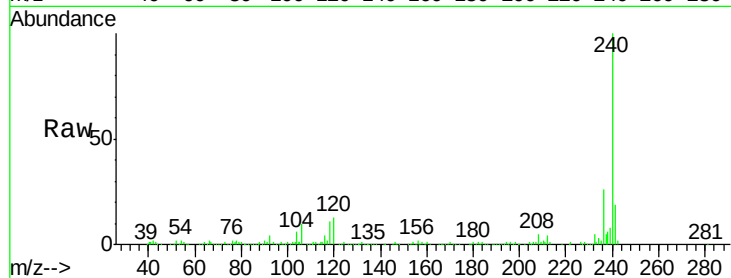

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

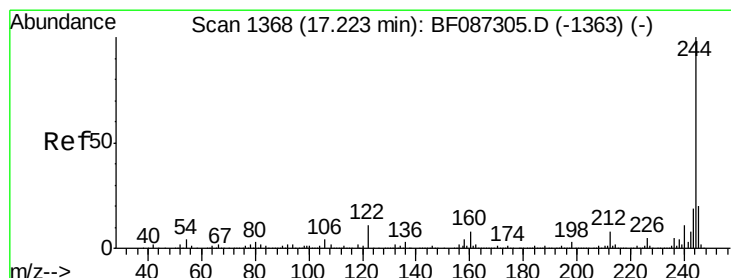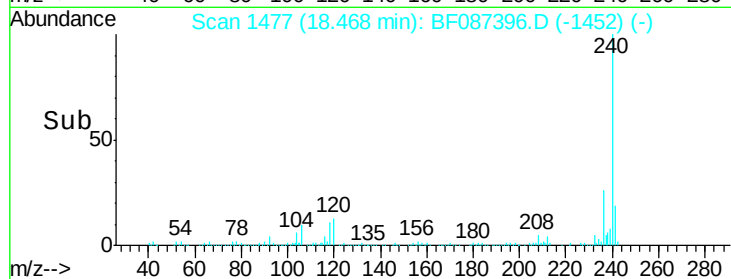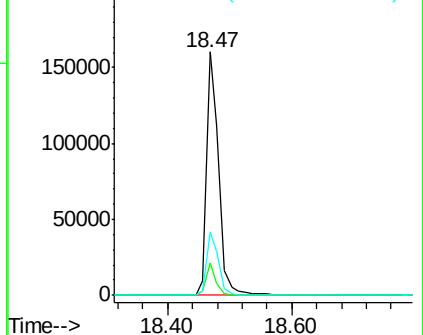

#78

Terphenyl-d14

Concen: 85.64 ng

RT: 17.13 min Scan# 1360

Delta R.T. -0.00 min

Lab File: BF087396.D

Acq: 26 May 2016 5:20


Tgt Ion:244 Resp: 866980

Ion Ratio Lower Upper

244 100

212 8.2 6.2 9.2



122 13.9 12.0 18.0

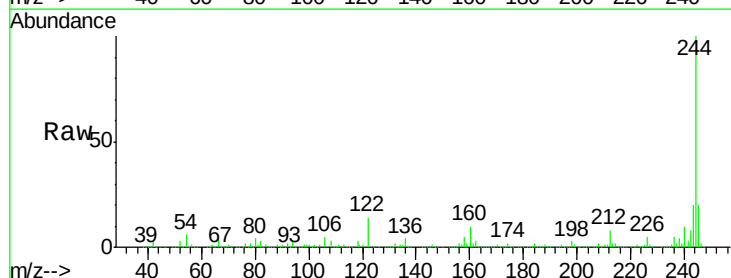


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

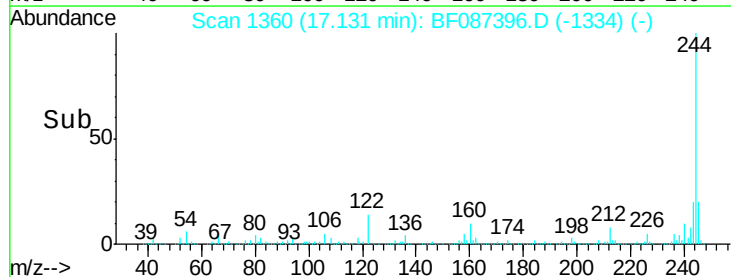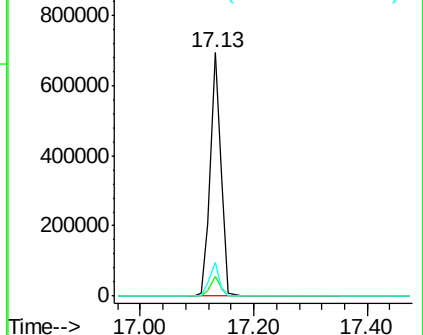

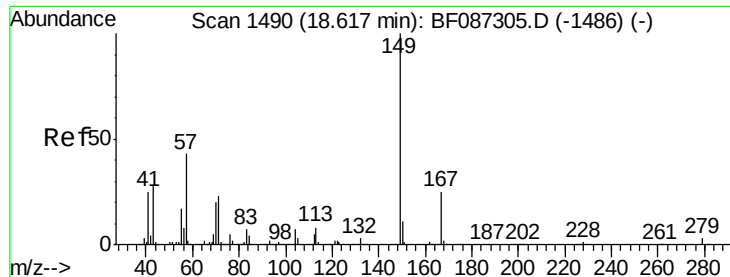

#83

Bis(2-ethylhexyl)phthalate

Concen: 2.70 ng

RT: 18.54 min Scan# 1483

Delta R.T. -0.00 min

Lab File: BF087396.D

Acq: 26 May 2016 5:20

Instrument :

BNA_F

ClientSampleId :

SB-34-COMP


Tot Ion:149 Resp: 27041

Ion Ratio Lower Upper

149 100

167 26.2 21.8 32.6




279 0.0 2.6 4.0#

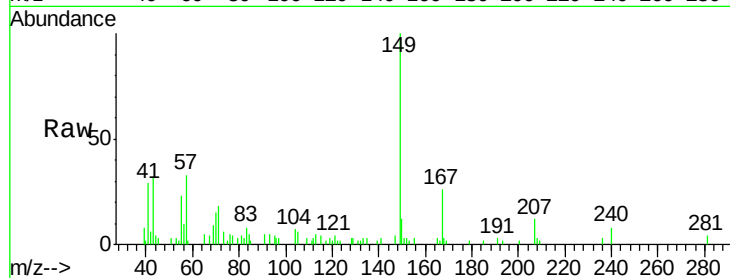

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

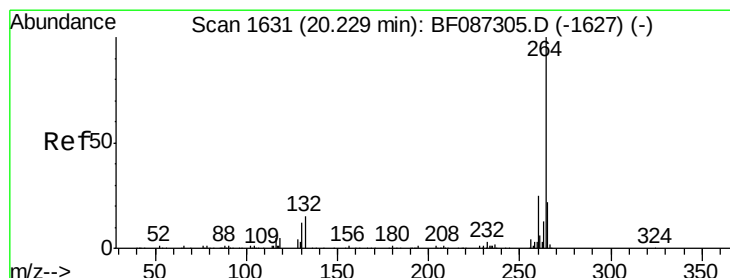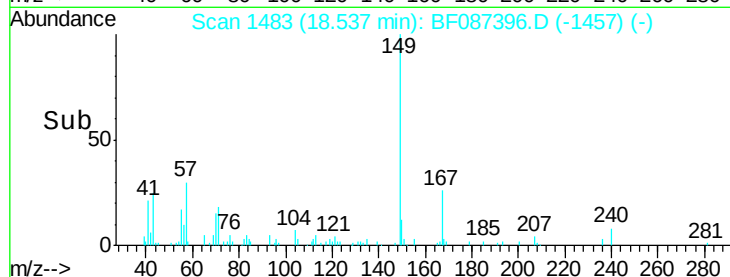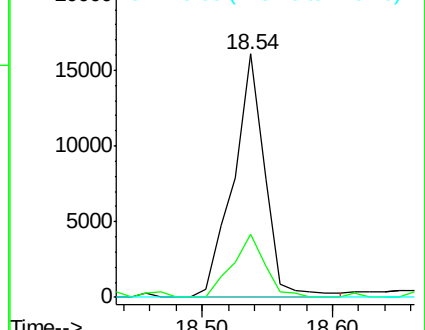

#86

Perylene-d12

Concen: 20.00 ng

RT: 20.14 min Scan# 1623

Delta R.T. -0.00 min

Lab File: BF087396.D

Acq: 26 May 2016 5:20


Tgt Ion:264 Resp: 143133

Ion Ratio Lower Upper

264 100

260 24.9 19.5 29.3

265 21.9 17.3 25.9

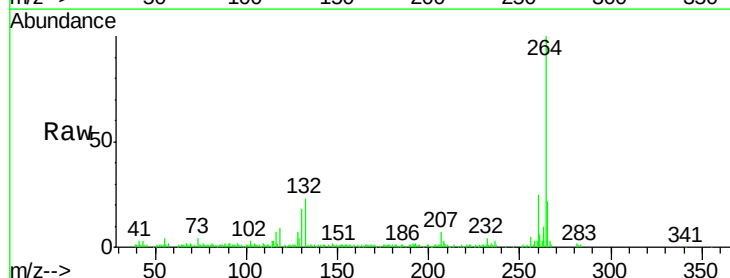

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

