


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052516\
 Data File : BF087385.D
 Acq On : 25 May 2016 23:03
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 25 16:26:52 2016

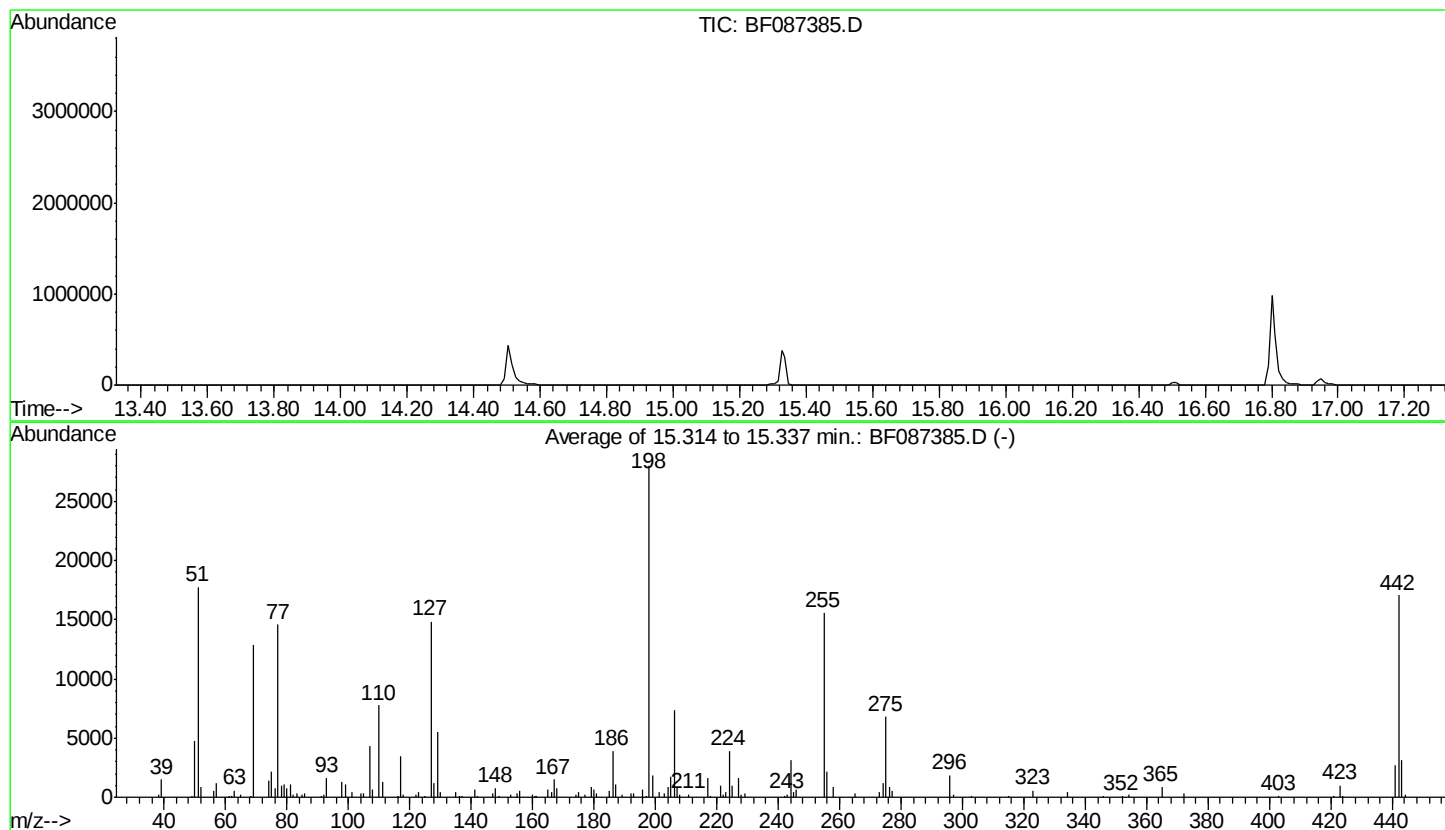

AutoFind: Scans 1201, 1202, 1203; Background Corrected with Scan 1198

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	63.4	17749	PASS
68	69	0.00	2	1.0	128	PASS
69	198	0.00	100	45.8	12821	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.9	14830	PASS
197	198	0.00	2	0.5	140	PASS
198	198	100	100	100.0	28016	PASS
199	198	5	9	6.6	1853	PASS
275	198	10	60	24.3	6799	PASS
365	198	1	100	3.2	891	PASS
441	442	0.01	24	15.9	2712	PASS
442	198	50	100	60.9	17067	PASS
443	442	15	24	18.5	3155	PASS