
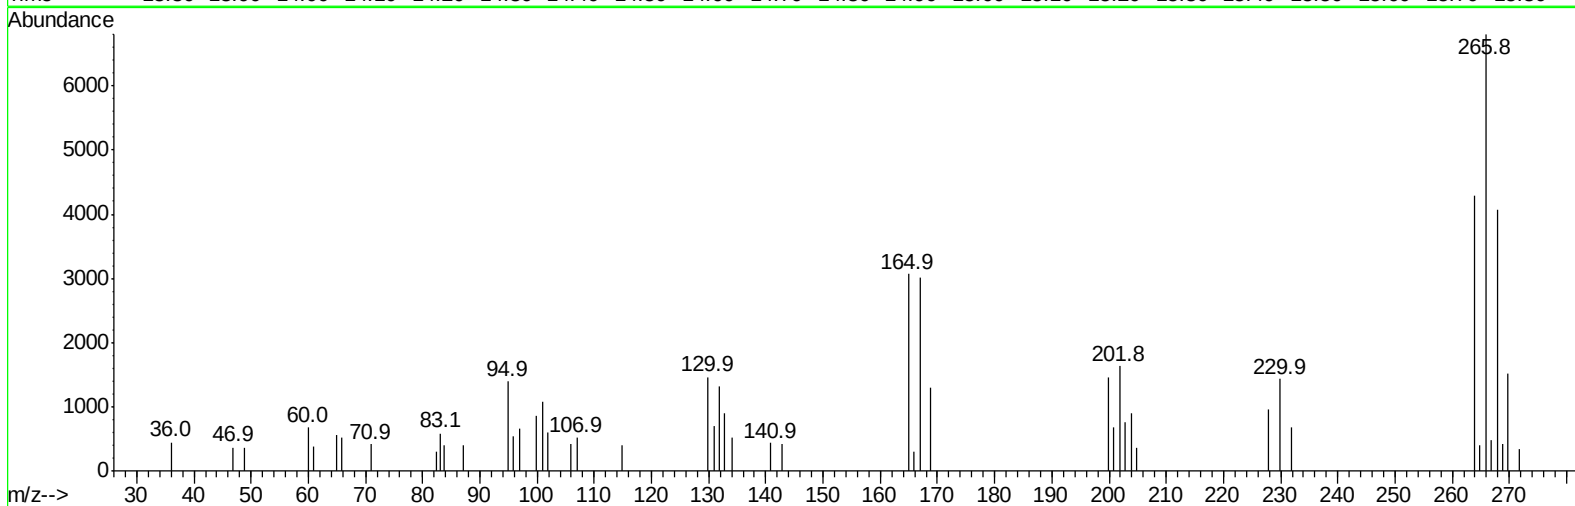


Data Path : Z:\HPCHEM1\BNA F\DATA\BF052517\
Data File : BF095446.D
Acq On : 26 May 2017 4:24
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 26 09:38:04 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 18 17:07:53 2017
Response via : Initial Calibration

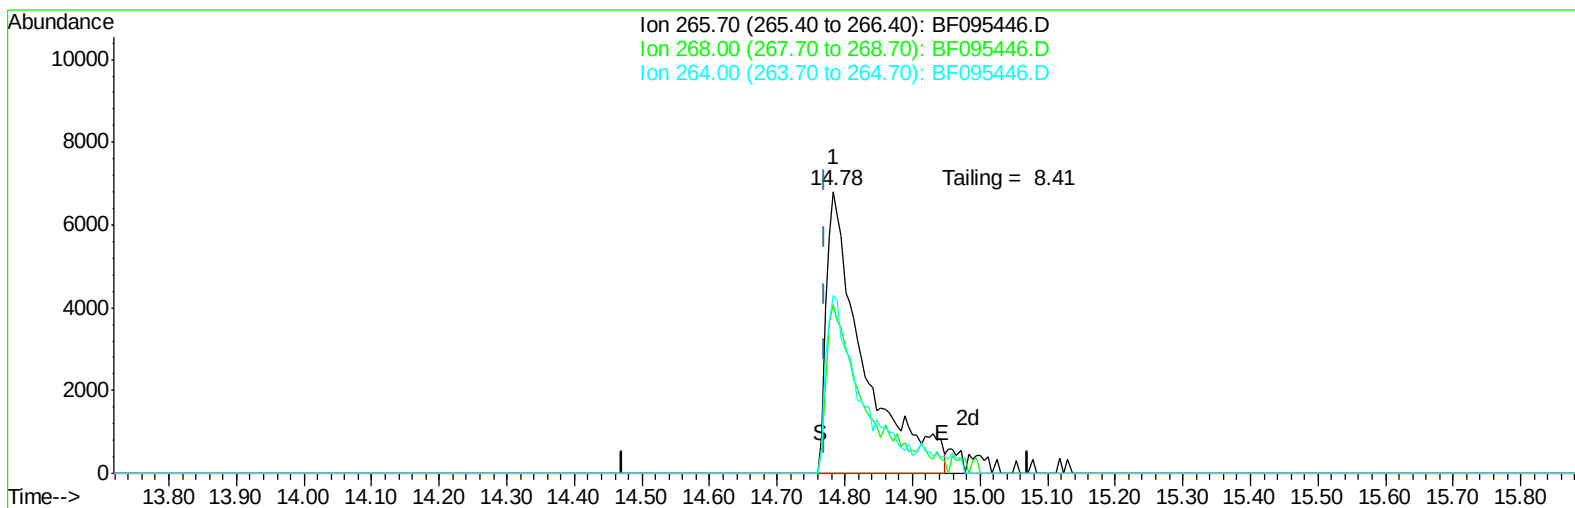

TIC: BF095446.D

(69) Pentachlorophenol (C)



14.783min (+0.012) 0.00ng

response 22499

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	59.88
264.00	64.60	63.04
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF052517\
Data File : BF095446.D
Acq On : 26 May 2017 4:24
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 26 09:38:04 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 18 17:07:53 2017
Response via : Initial Calibration

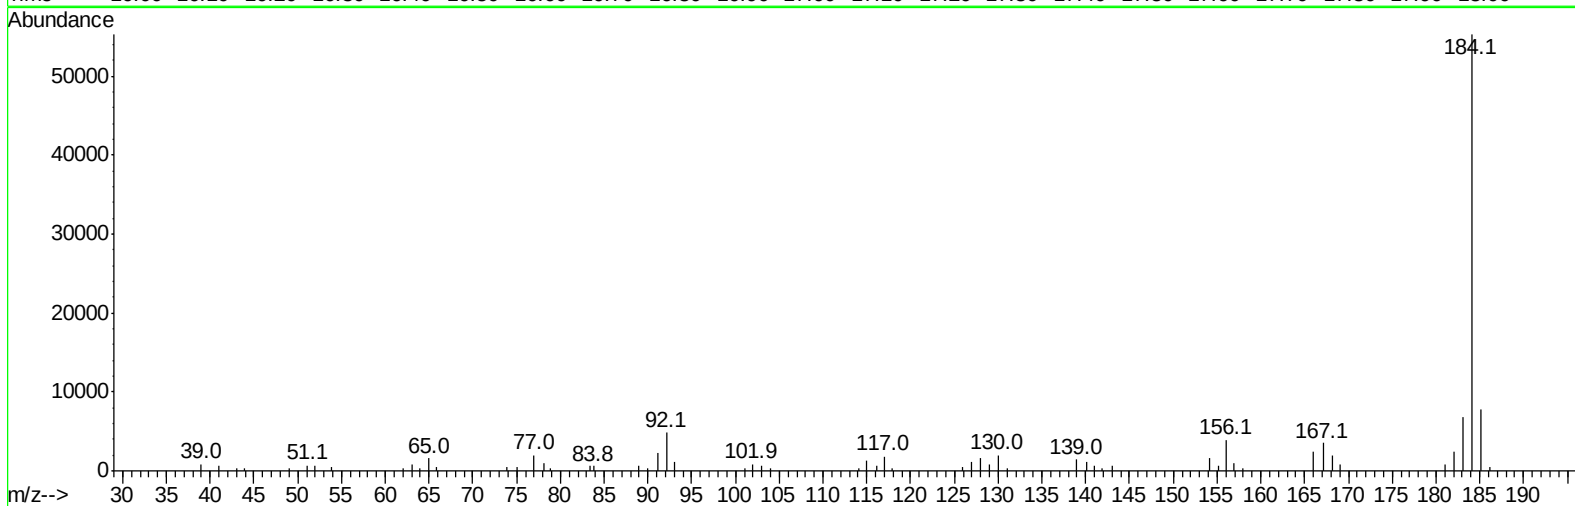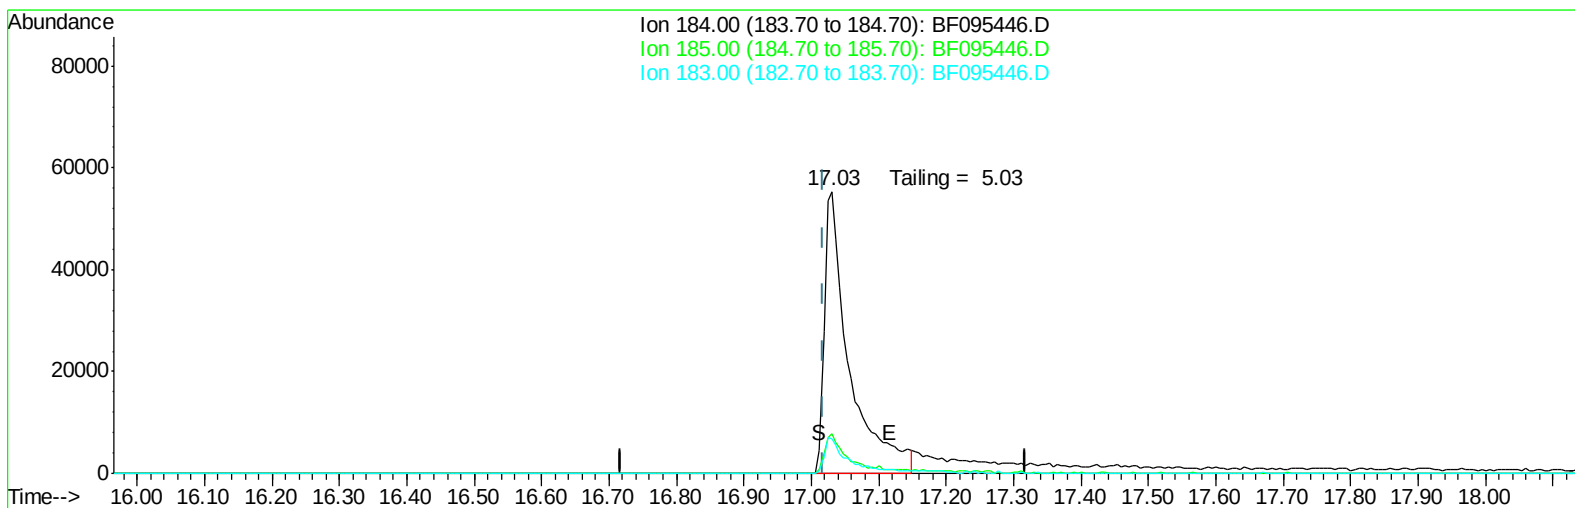

TIC: BF095446.D

(76) Benzidine

17.030min (+0.012) 0.00ng

response 138783

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.06#
183.00	12.20	12.26
0.00	0.00	0.00