


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052523\
Data File : BF133482.D
Acq On : 25 May 2023 10:25
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu May 25 23:30:55 2023

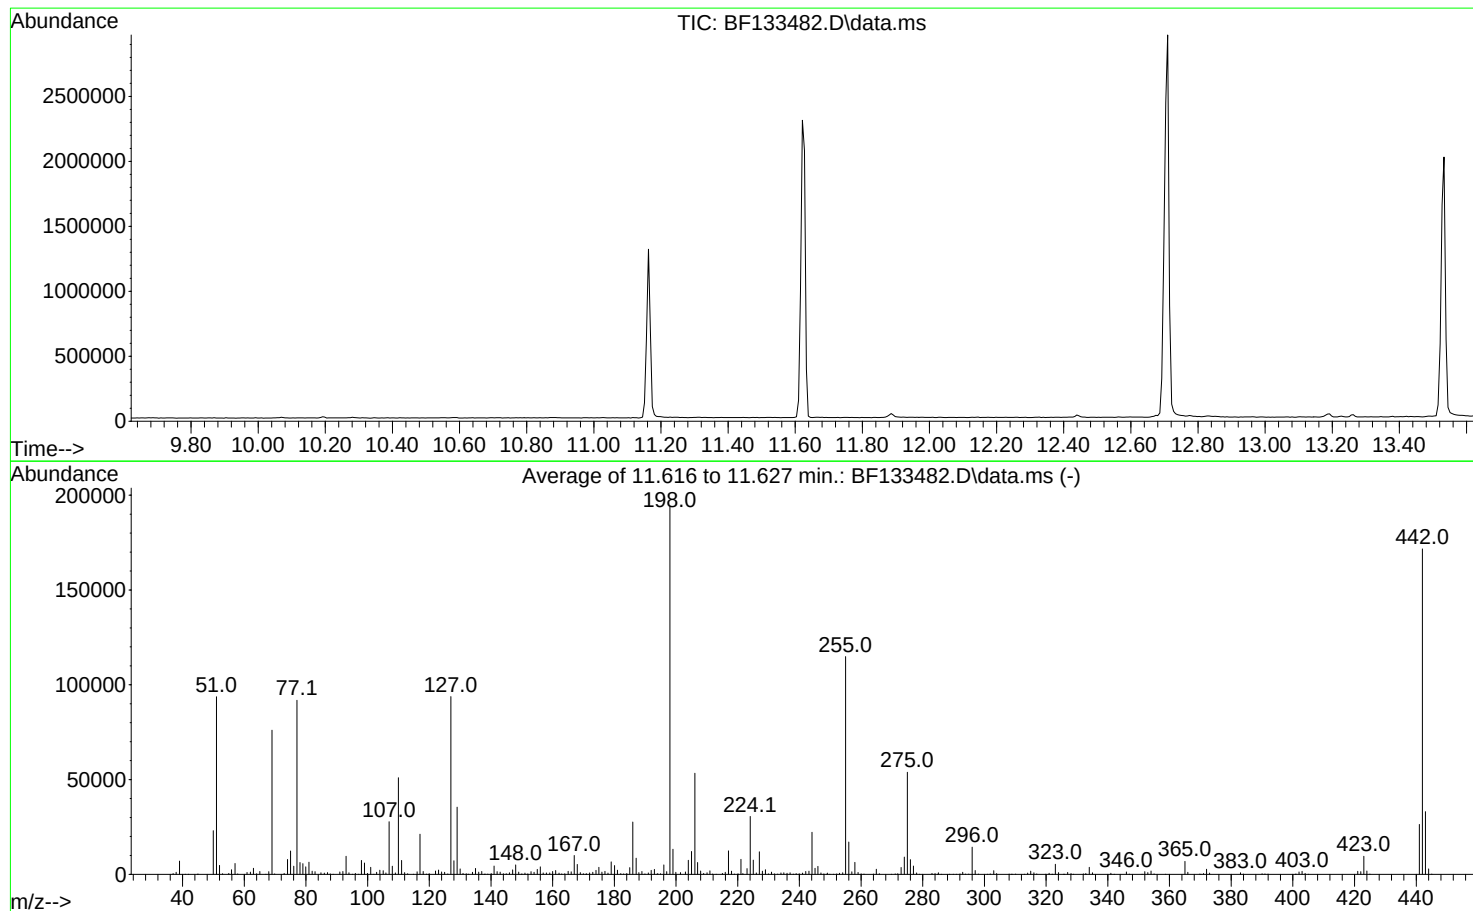

AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.3	93675	PASS
68	69	0.00	2	1.9	1439	PASS
69	198	0.00	100	39.2	76077	PASS
70	69	0.00	2	0.3	257	PASS
127	198	10	80	48.3	93784	PASS
197	198	0.00	2	0.7	1408	PASS
198	198	100	100	100.0	194043	PASS
199	198	5	9	6.8	13277	PASS
275	198	10	60	27.8	53851	PASS
365	198	1	100	3.5	6880	PASS
441	198	0.01	100	13.6	26374	PASS
442	442	50	100	100.0	171704	PASS
443	442	15	24	19.3	33096	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/25/2023	BNA_F	<u>BF133482.D</u>
Compound Name	Response	Retention Time
DDT	258241	13.533
DDD	3075	13.263
DDE	0	12.896
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3075	261316	1.18

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052523\
Data File : BF133482.D
Acq On : 25 May 2023 10:25
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 26 06:13:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 25 23:30:55 2023
Response via : Initial Calibration

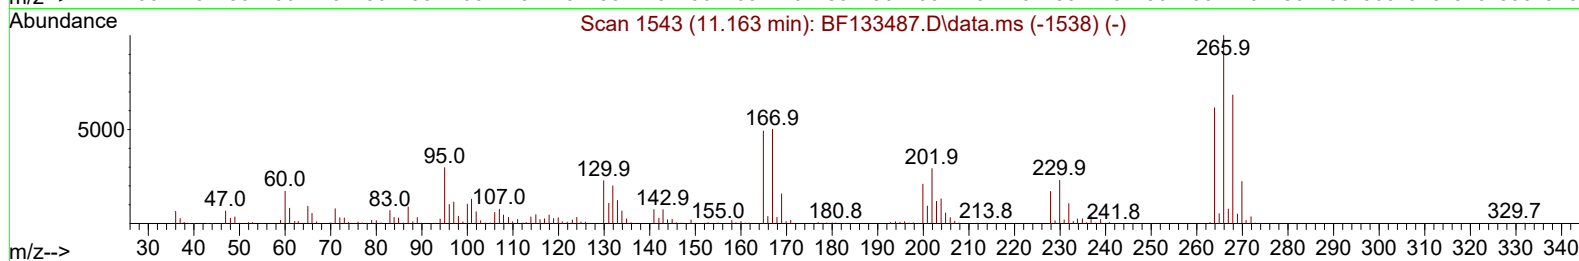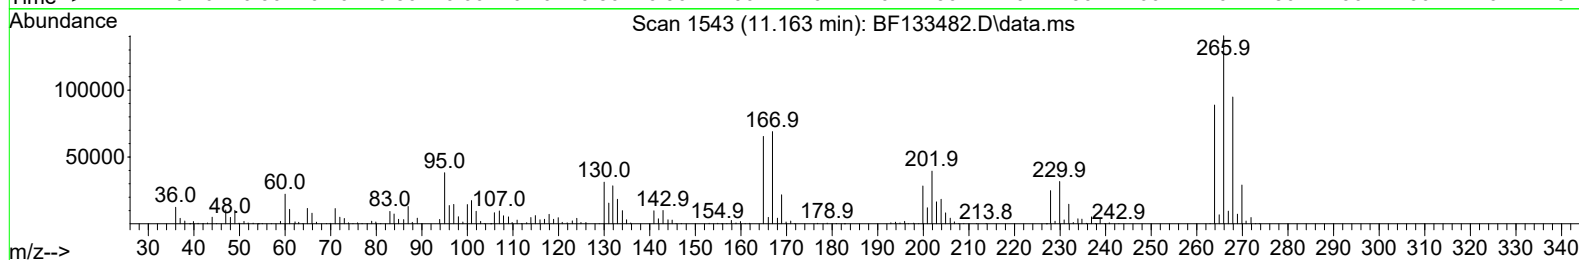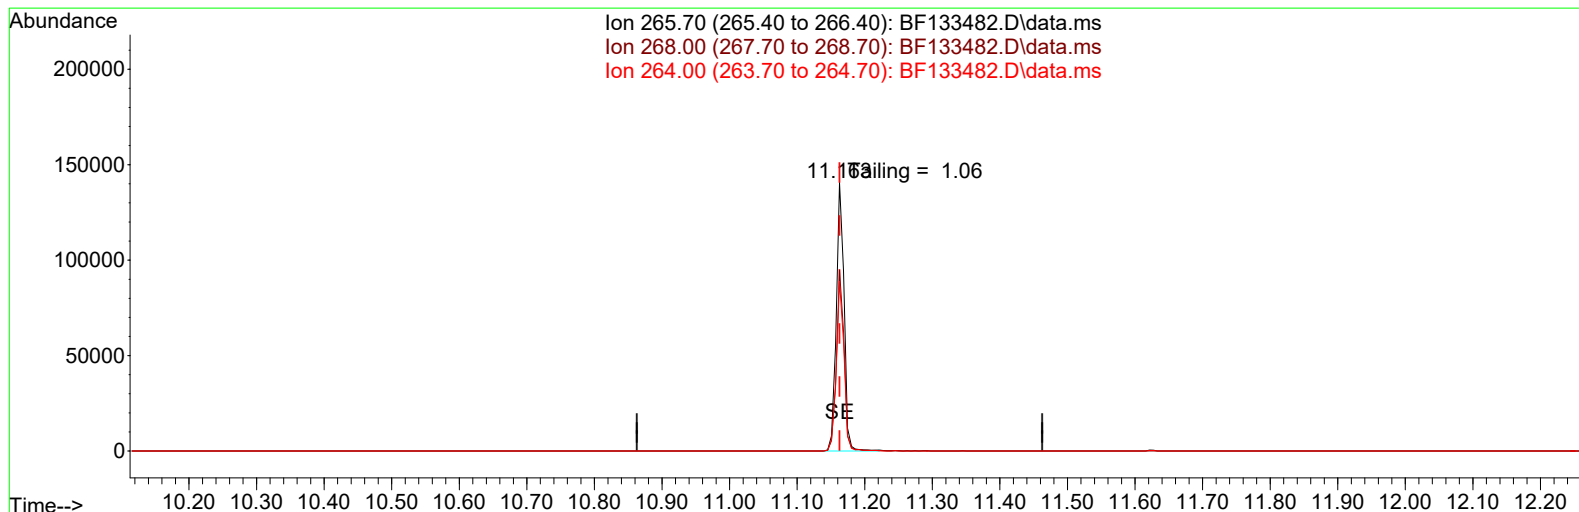

TIC: BF133482.D\data.ms

(70) Pentachlorophenol (C)

11.163min (-0.000) 17581.07 ng




response 112194

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	68.30	67.42
264.00	61.50	63.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052523\
Data File : BF133482.D
Acq On : 25 May 2023 10:25
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 26 06:13:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 25 23:30:55 2023
Response via : Initial Calibration

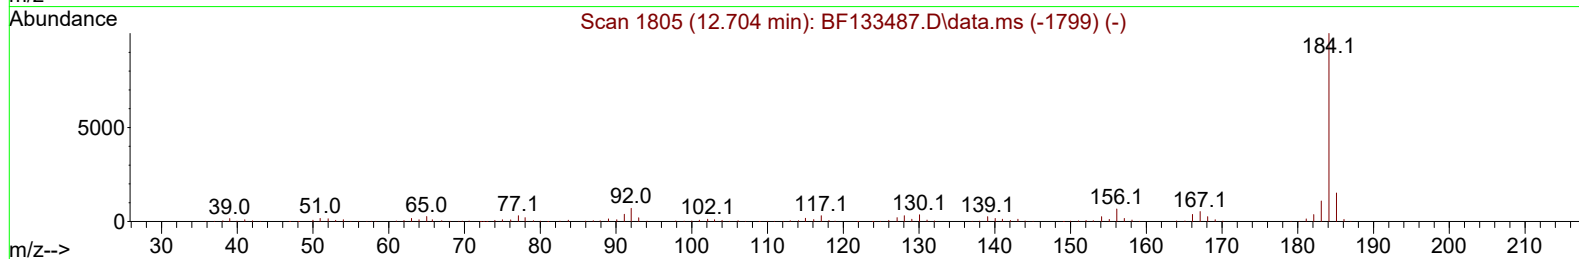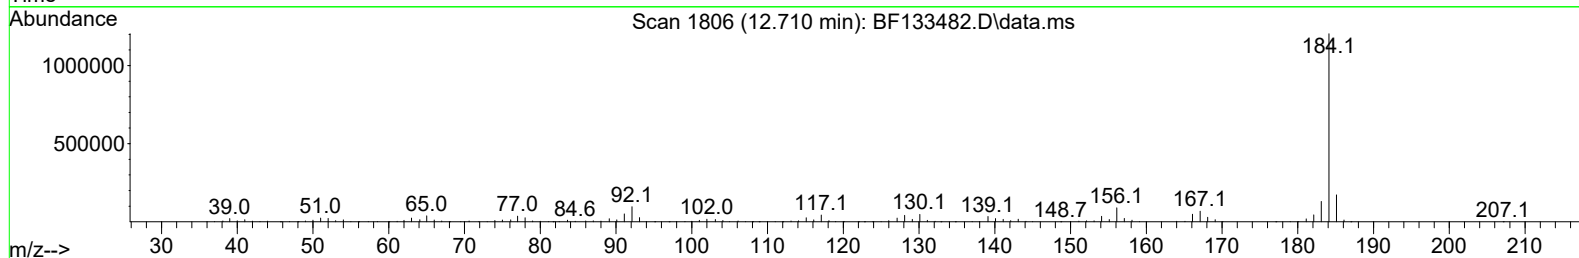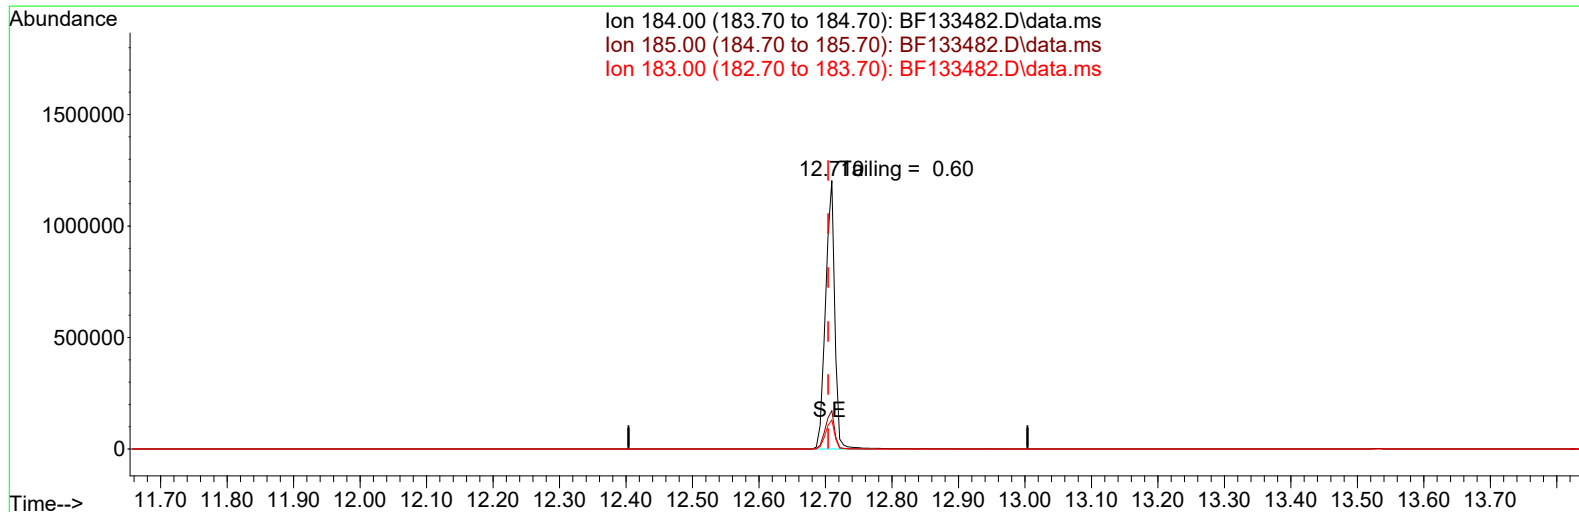

TIC: BF133482.D\data.ms

(77) Benzidine

12.710min (+ 0.006) 0.00 ng

response 1158211

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.32
183.00	10.90	10.84
0.00	0.00	0.00