
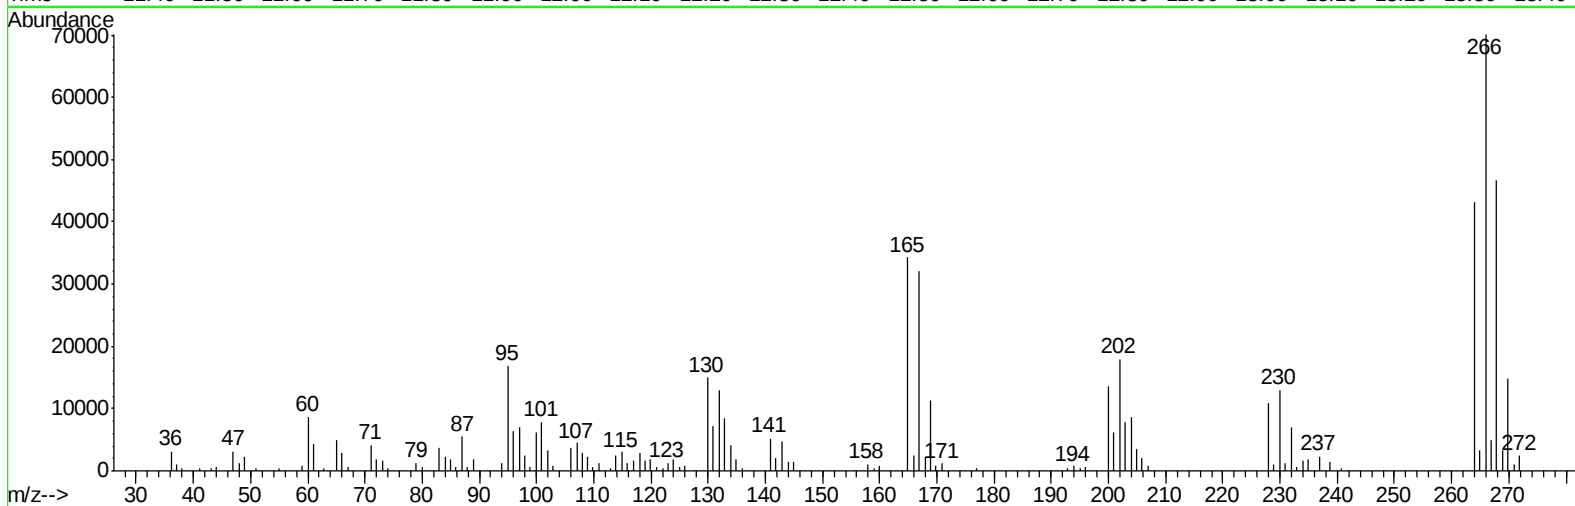


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052615\
Data File : BF079509.D
Acq On : 27 May 2015 8:06
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 27 08:58:09 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 27 07:31:10 2015
Response via : Initial Calibration

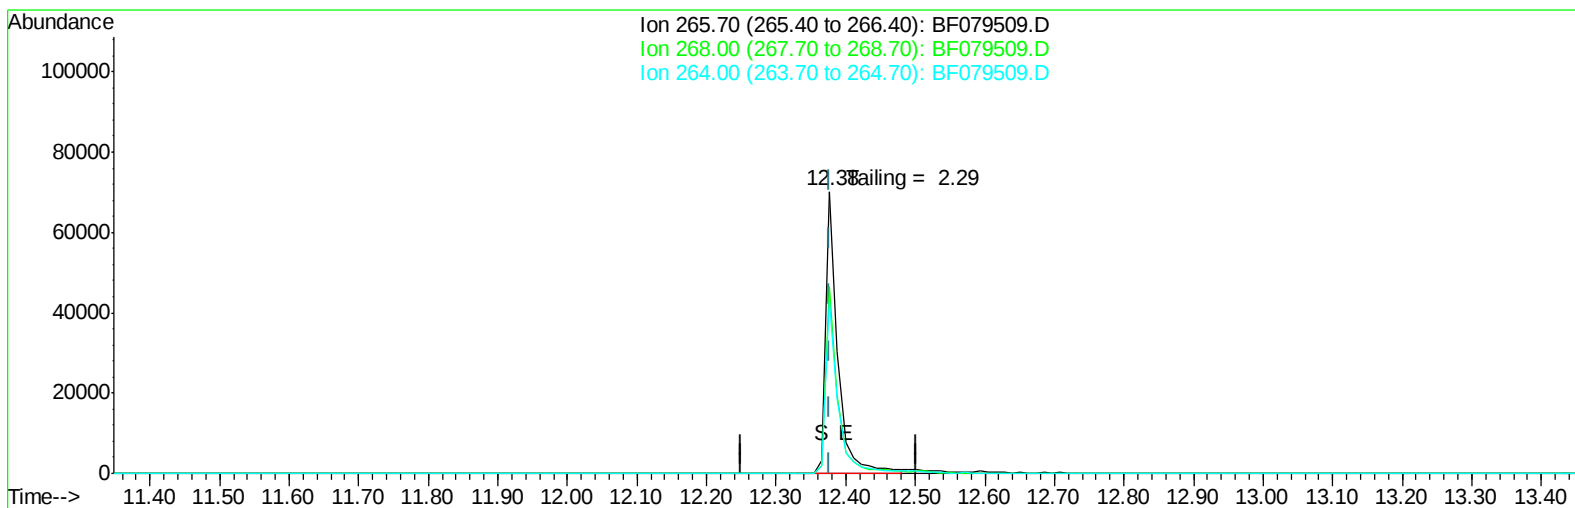

TIC: BF079509.D

(69) Pentachlorophenol (C)

12.377min (+0.000) 0.00ng

response 83306

Ion	Exp%	Act%
265.70	100	100
268.00	70.10	66.59
264.00	62.50	61.49
0.00	0.00	0.00