
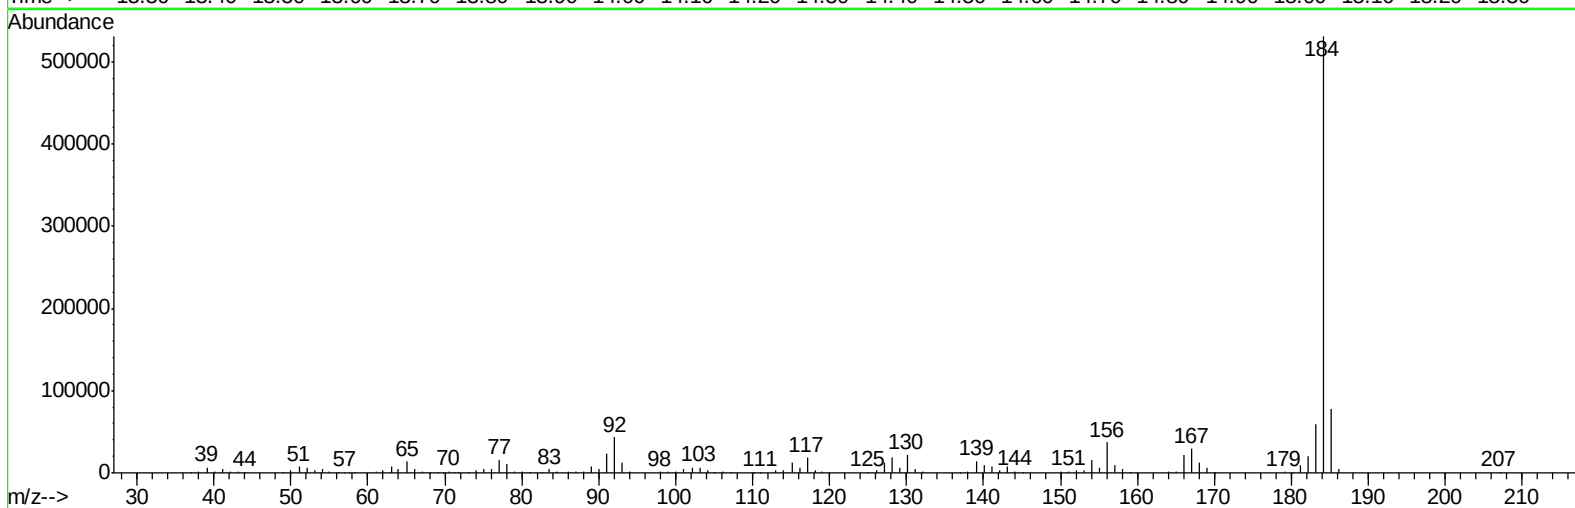


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052615\
Data File : BF079509.D
Acq On : 27 May 2015 8:06
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 27 08:58:09 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 27 07:31:10 2015
Response via : Initial Calibration

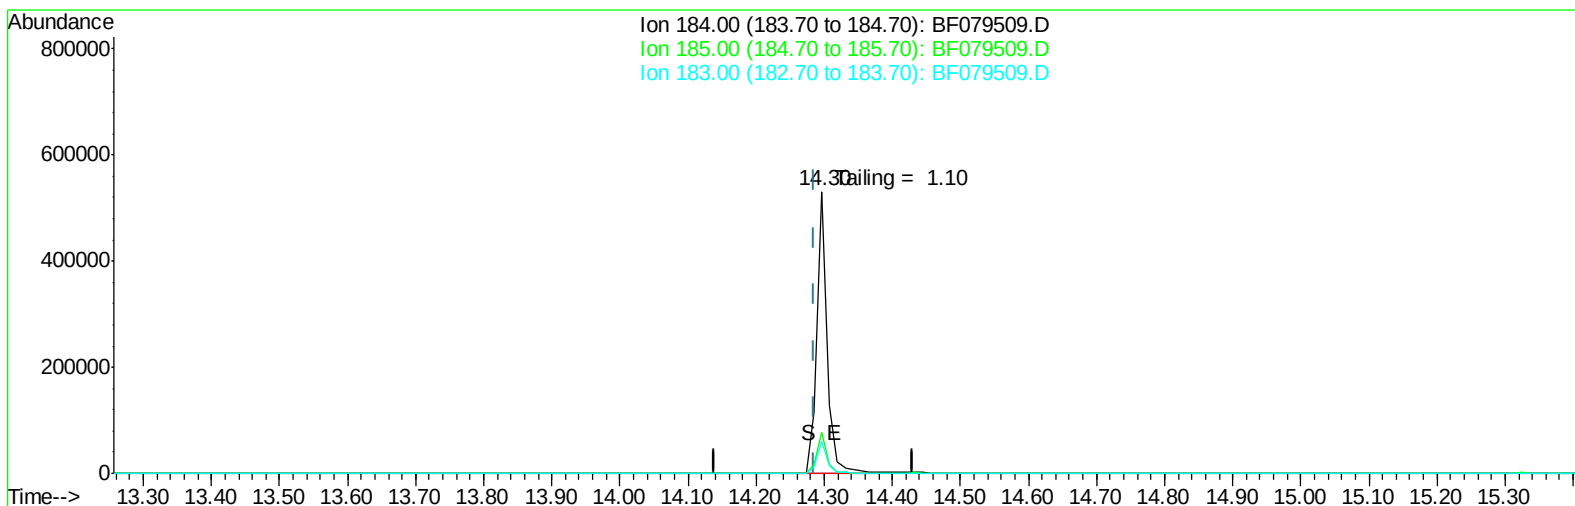

TIC: BF079509.D

(76) Benzidine

14.297min (+0.012) 25734.81ng

response 569950

Ion	Exp%	Act%
184.00	100	100
185.00	15.10	14.60
183.00	10.70	11.28
0.00	0.00	0.00