


Data Path : Z:\HPCHEM1\BNA_F\Data\BF052615\
 Data File : BF079486.D
 Acq On : 26 May 2015 19:57
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052615.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 27 01:32:46 2015

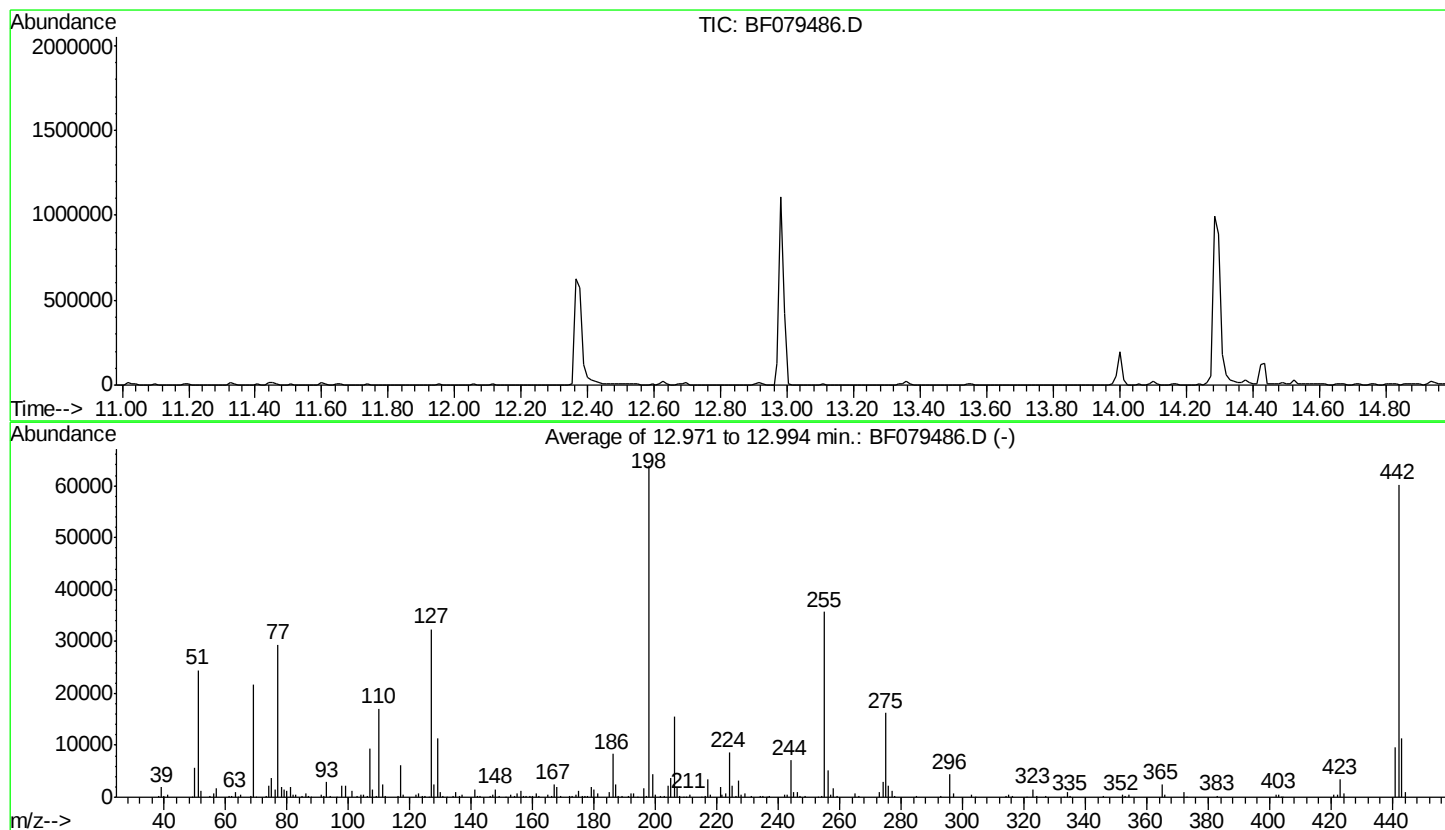

AutoFind: Scans 1031, 1032, 1033; Background Corrected with Scan 1028

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.3	24468	PASS
68	69	0.00	2	1.3	278	PASS
69	198	0.00	100	34.1	21777	PASS
70	69	0.00	2	0.5	111	PASS
127	198	10	80	50.7	32384	PASS
197	198	0.00	2	0.5	288	PASS
198	198	100	100	100.0	63874	PASS
199	198	5	9	7.0	4468	PASS
275	198	10	60	25.4	16230	PASS
365	198	1	100	3.7	2379	PASS
441	442	0.01	24	15.8	9544	PASS
442	198	50	100	94.4	60267	PASS
443	442	15	24	19.0	11456	PASS