


Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF052615\  
 Data File : BF079509.D  
 Acq On : 27 May 2015 8:06  
 Operator : TP/IZ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF052615.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed May 27 07:31:10 2015

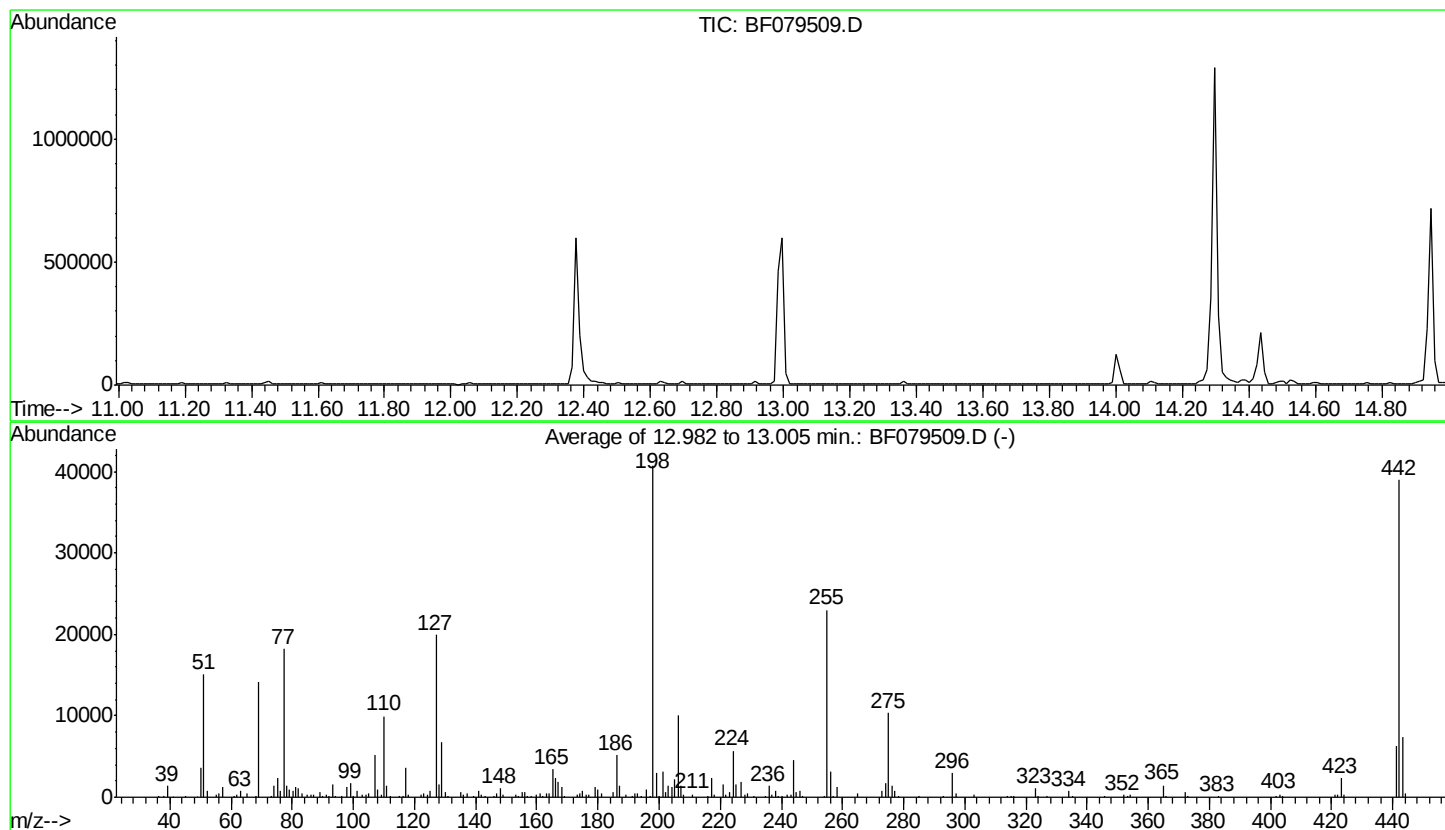

AutoFind: Scans 1032, 1033, 1034; Background Corrected with Scan 1028

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 37.0      | 15061   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.1       | 151     | PASS             |
| 69          | 198          | 0.00         | 100          | 34.6      | 14088   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 10           | 80           | 49.0      | 19966   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.3       | 132     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 40729   | PASS             |
| 199         | 198          | 5            | 9            | 7.3       | 2987    | PASS             |
| 275         | 198          | 10           | 60           | 25.4      | 10354   | PASS             |
| 365         | 198          | 1            | 100          | 3.6       | 1467    | PASS             |
| 441         | 442          | 0.01         | 24           | 16.1      | 6254    | PASS             |
| 442         | 198          | 50           | 100          | 95.6      | 38955   | PASS             |
| 443         | 442          | 15           | 24           | 19.1      | 7427    | PASS             |