
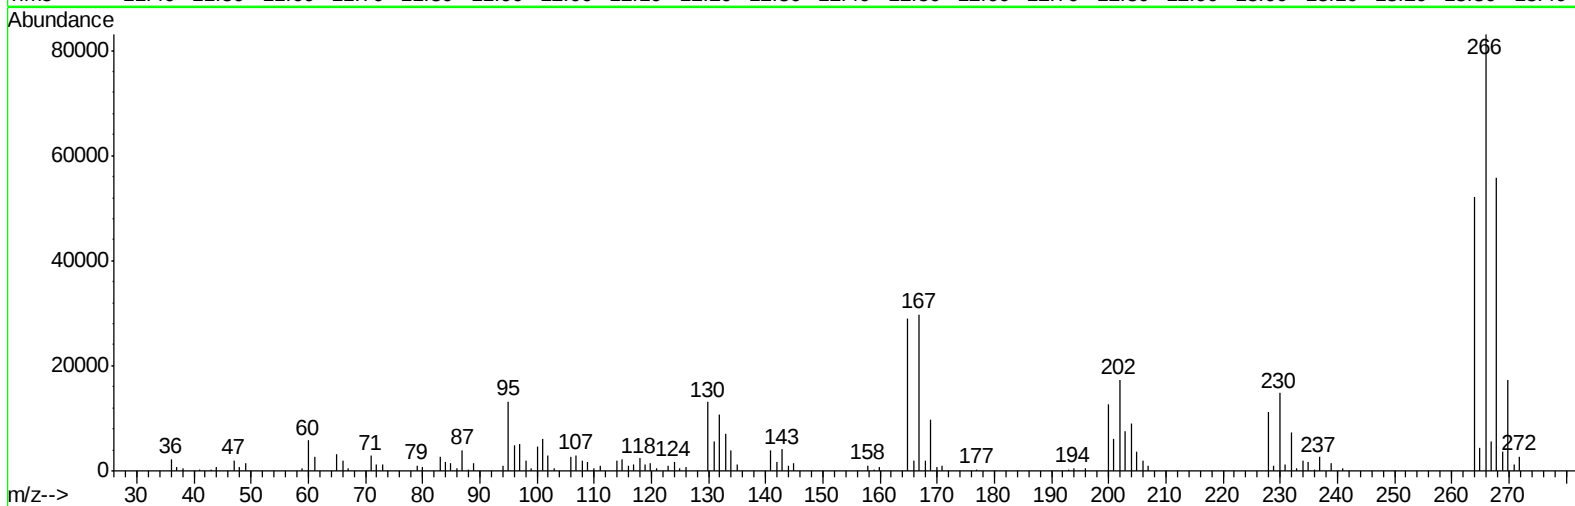


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052615\
Data File : BF079486.D
Acq On : 26 May 2015 19:57
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 27 07:30:30 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 27 01:32:46 2015
Response via : Initial Calibration

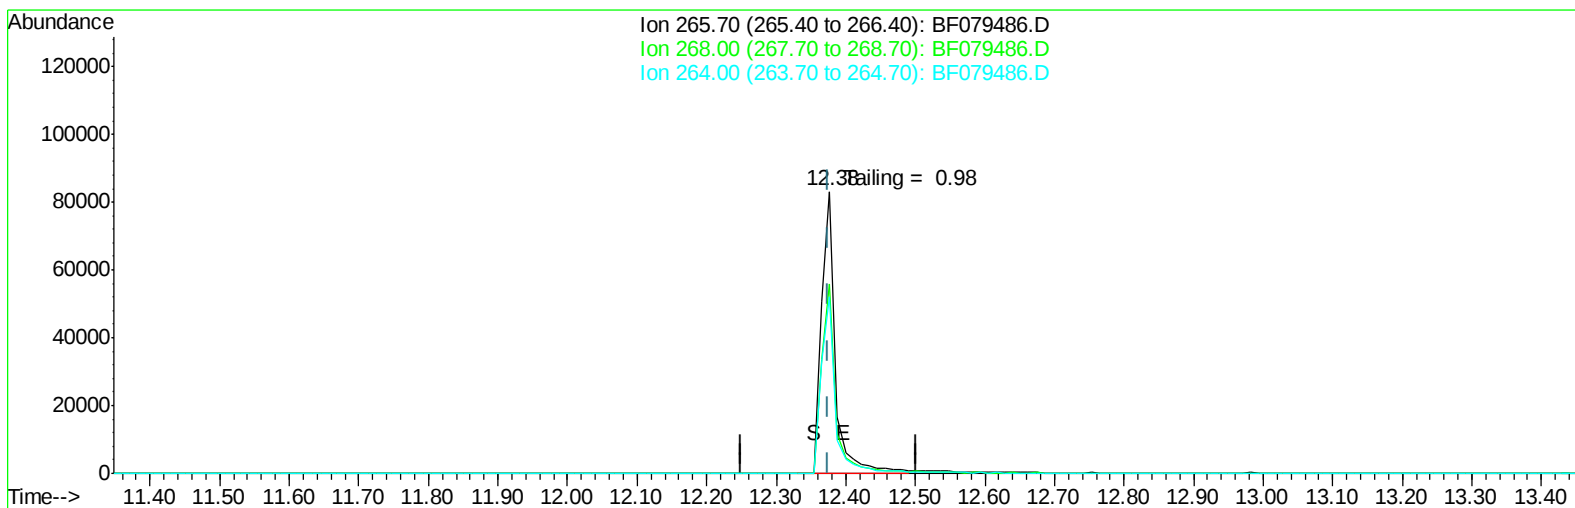

TIC: BF079486.D

(69) Pentachlorophenol (C)



12.376min (+0.000) 0.00ng

response 115515

Ion	Exp%	Act%
265.70	100	100
268.00	70.10	67.06
264.00	62.50	62.78
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052615\
Data File : BF079486.D
Acq On : 26 May 2015 19:57
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 27 07:30:30 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 27 01:32:46 2015
Response via : Initial Calibration

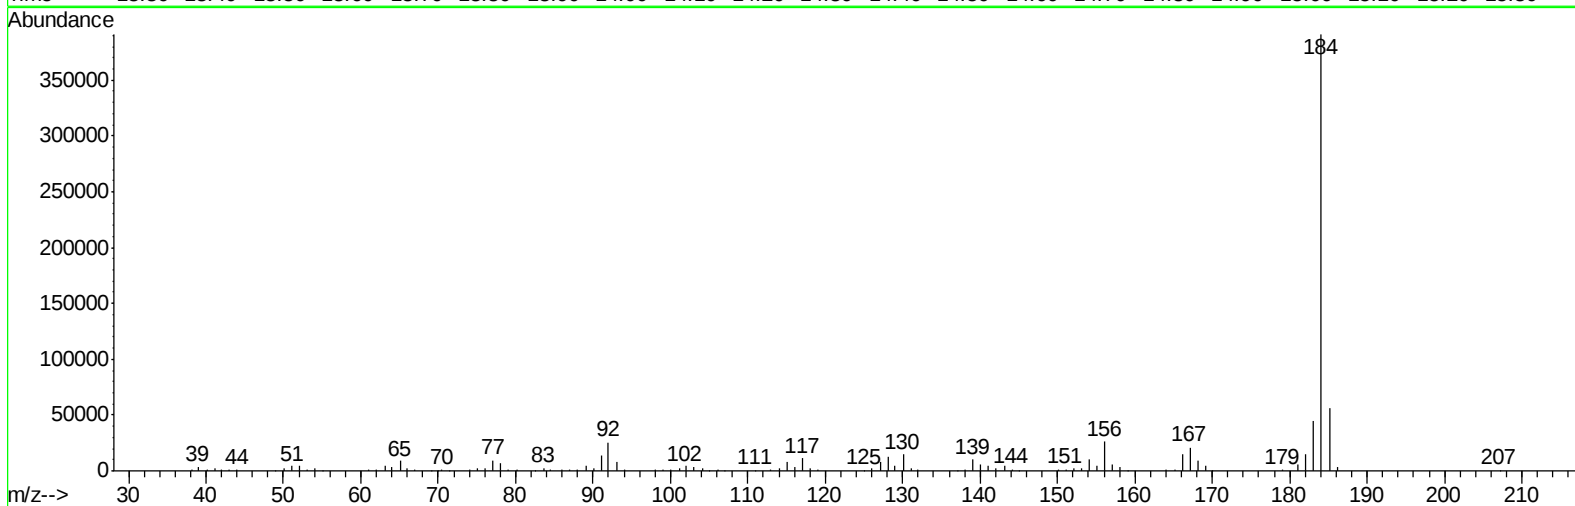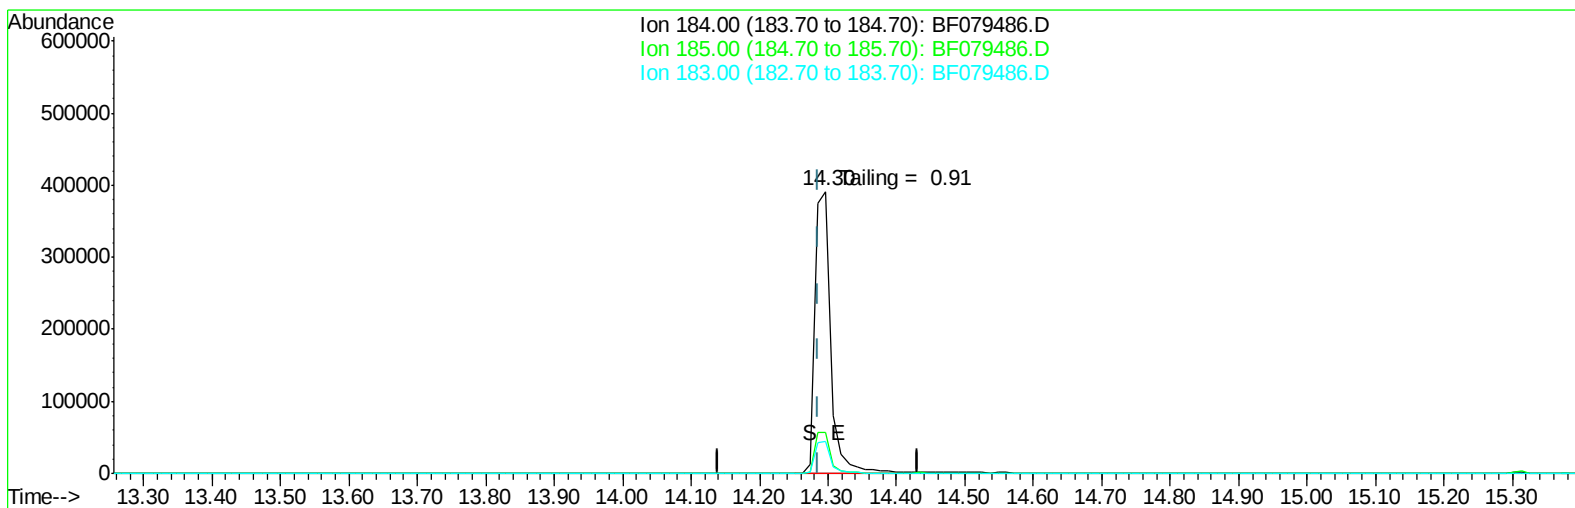

TIC: BF079486.D

(76) Benzidine

14.297min (+0.012) 38032.95ng

response 635404

Ion	Exp%	Act%
184.00	100	100
185.00	15.10	14.44
183.00	10.70	11.44
0.00	0.00	0.00