

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052615\
 Data File : BF079488.D
 Acq On : 26 May 2015 21:23
 Operator : TP/IZ
 Sample : G2362-01RE
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FK-GF-01-015-ARE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052615.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.290	7	9	20	rVB2	167187	470028	6.67%	1.214%
2	1.450	20	23	29	rVV	341739	512705	7.27%	1.325%
3	1.587	34	35	43	rVV	622236	988294	14.02%	2.553%
4	1.701	43	45	81	rVB	3003186	7048381	100.00%	18.210%
5	4.741	310	311	321	rBV	138376	243545	3.46%	0.629%
6	5.301	358	360	373	rBV	2011846	2274696	32.27%	5.877%
7	6.616	472	475	477	rBV	2165181	2431166	34.49%	6.281%
8	6.730	483	485	488	rBV	2184950	2407229	34.15%	6.219%
9	7.016	507	510	513	rBV	782580	727230	10.32%	1.879%
10	7.199	524	526	529	rBV	1848467	1832111	25.99%	4.733%
11	7.713	569	571	574	rBV	1451761	1438060	20.40%	3.715%
12	8.593	646	648	651	rBV	1143890	1030013	14.61%	2.661%
13	9.942	764	766	768	rBV	3207133	2837125	40.25%	7.330%
14	10.456	809	811	813	rBV	159503	188234	2.67%	0.486%
15	10.731	829	835	836	rBV2	59806	120869	1.71%	0.312%
16	10.765	836	838	840	rVB	868951	1146985	16.27%	2.963%
17	11.736	921	923	926	rBV2	1565148	1995402	28.31%	5.155%
18	11.942	939	941	945	rBV	72240	106344	1.51%	0.275%
19	12.594	996	998	1000	rBV	1199154	1248915	17.72%	3.227%
20	13.337	1060	1063	1067	rBV2	105611	207893	2.95%	0.537%
21	14.102	1127	1130	1132	rVB	187472	230440	3.27%	0.595%
22	14.377	1152	1154	1156	rVB	221791	259601	3.68%	0.671%
23	14.594	1170	1173	1175	rBV	2933322	3275893	46.48%	8.464%
24	15.760	1273	1275	1279	rBV	364627	521224	7.39%	1.347%
25	15.874	1282	1285	1287	rBV	1219346	1505803	21.36%	3.890%
26	16.560	1343	1345	1350	rVB2	55591	109288	1.55%	0.282%
27	17.017	1383	1385	1387	rVB	87915	97099	1.38%	0.251%
28	17.131	1393	1395	1401	rBV	124311	308246	4.37%	0.796%
29	17.326	1409	1412	1415	rBV4	57225	146364	2.08%	0.378%
30	17.440	1420	1422	1424	rBV	86682	115831	1.64%	0.299%
31	17.508	1426	1428	1430	rBV	104915	148824	2.11%	0.385%
32	17.566	1430	1433	1436	rBV	1141693	1380038	19.58%	3.565%
33	17.691	1442	1444	1447	rBV3	48490	81697	1.16%	0.211%
34	18.194	1486	1488	1495	rVB	125518	253935	3.60%	0.656%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052615\
Data File : BF079488.D
Acq On : 26 May 2015 21:23
Operator : TP/IZ
Sample : G2362-01RE
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FK-GF-01-015-ARE

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052615.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	18.571	1519	1521	1530	rVB2	134694	297769	4.22%	0.769%
36	18.891	1546	1549	1555	rVB2	67934	177791	2.52%	0.459%
37	19.269	1580	1582	1585	rBV	56979	81862	1.16%	0.212%
38	19.406	1591	1594	1598	rVB5	57357	129787	1.84%	0.335%
39	21.143	1743	1746	1751	rVB	116530	328649	4.66%	0.849%


Sum of corrected areas: 38705366

Data Path : Z:\HPCHEM1\BNA F\DATA\BF052615\
Data File : BF079488.D
Acq On : 26 May 2015 21:23
Operator : TP/IZ
Sample : G2362-01RE
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FK-GF-01-015-ARE

Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF052615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

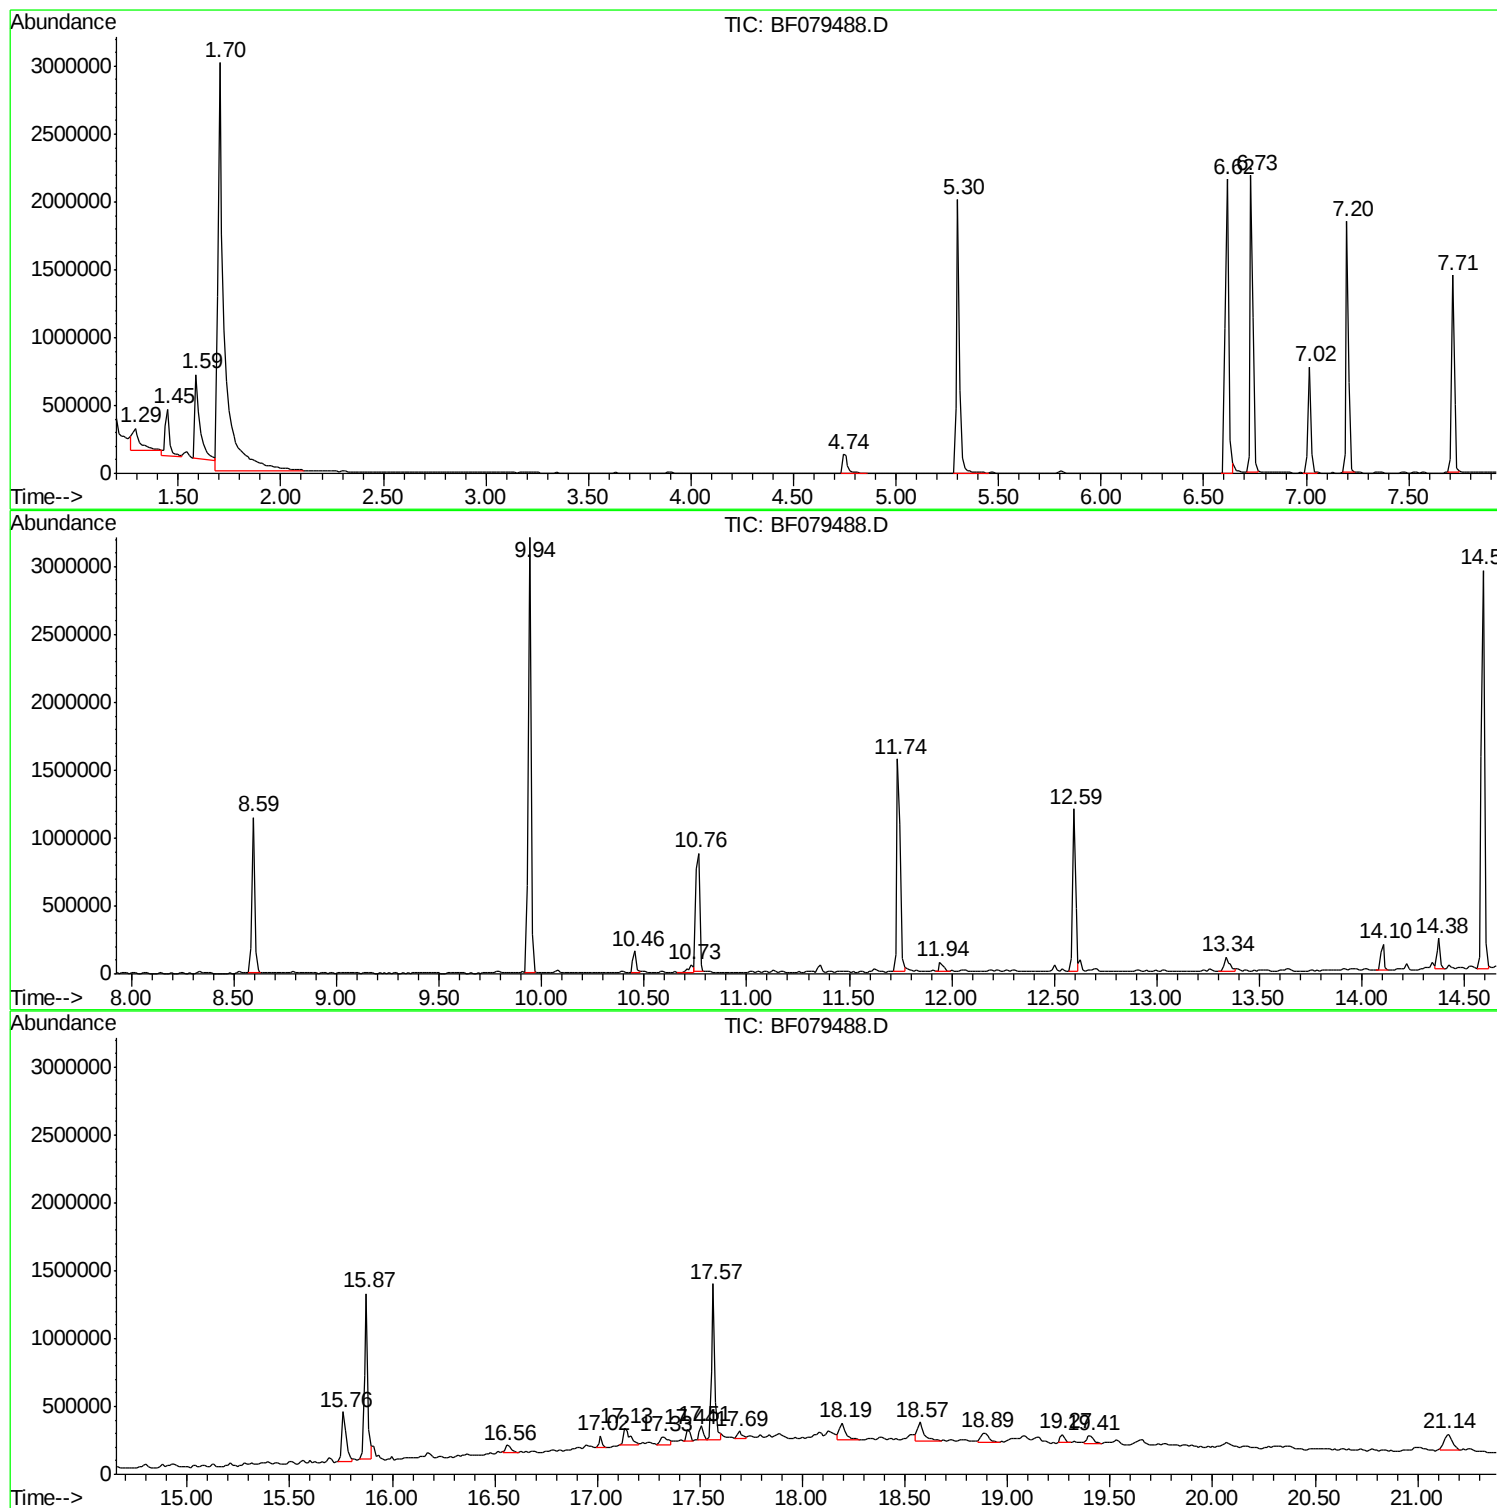

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF052615\
Data_File : BF079488.D
Acq_On : 26 May, 2015 21:233
Operator : TP/IZZ
Sample : G2362-01REE
Misc :
ALS_Vial : 11 Sample Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
FK-GF-01-015-ARE

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052615.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION.NN

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
