

Data Path : Z:\HPCHEM1\BNA F\DATA\BF052615\
 Data File : BF079489.D
 Acq On : 26 May 2015 21:52
 Operator : TP/IZ
 Sample : G2362-03RE
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FK-GF-01-015-BRE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052615.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	7	10	21	rVB2	129906	390835	8.23%	0.980%
2	1.461	21	24	30	rVV	286943	468596	9.87%	1.175%
3	1.541	30	31	34	rVV	44487	63132	1.33%	0.158%
4	1.587	34	35	43	rVV	447518	712247	15.00%	1.786%
5	1.701	43	45	78	rVB	2172999	4749387	100.00%	11.912%
6	4.753	310	312	321	rVB	192298	303926	6.40%	0.762%
7	5.301	358	360	373	rBV	1899331	2771385	58.35%	6.951%
8	6.616	473	475	483	rBV	2798650	2889871	60.85%	7.248%
9	6.730	483	485	488	rBV	2177672	2947907	62.07%	7.394%
10	7.016	508	510	513	rBV	891254	830223	17.48%	2.082%
11	7.199	524	526	529	rBV	1942979	2072734	43.64%	5.199%
12	7.713	569	571	574	rBV	1502546	1749939	36.85%	4.389%
13	8.593	646	648	651	rBV	1272027	1152362	24.26%	2.890%
14	9.942	764	766	769	rBV	3184271	2879686	60.63%	7.223%
15	10.456	809	811	813	rBV	281760	294584	6.20%	0.739%
16	10.731	830	835	836	rBV2	50083	103376	2.18%	0.259%
17	10.765	836	838	840	rVB	1155776	1309415	27.57%	3.284%
18	11.359	888	890	892	rVB	63156	61482	1.29%	0.154%
19	11.748	921	924	926	rBV2	1645820	2393402	50.39%	6.003%
20	11.942	939	941	946	rBV	70177	95827	2.02%	0.240%
21	12.594	996	998	1000	rBV	1254476	1375025	28.95%	3.449%
22	12.696	1003	1007	1010	rBV2	22808	62880	1.32%	0.158%
23	13.336	1060	1063	1073	rBV2	197501	359986	7.58%	0.903%
24	14.102	1127	1130	1132	rBV	150458	175406	3.69%	0.440%
25	14.217	1139	1140	1144	rVB4	50665	63955	1.35%	0.160%
26	14.319	1144	1149	1150	rBV3	30451	66464	1.40%	0.167%
27	14.377	1152	1154	1156	rVB	183189	209820	4.42%	0.526%
28	14.434	1156	1159	1161	rBV	181107	240489	5.06%	0.603%
29	14.594	1170	1173	1176	rBV	3293244	3389802	71.37%	8.502%
30	15.314	1233	1236	1238	rBV	167459	196083	4.13%	0.492%
31	15.771	1273	1276	1282	rBV	393054	704784	14.84%	1.768%
32	15.874	1282	1285	1287	rBV	1341685	1577267	33.21%	3.956%
33	16.182	1310	1312	1314	rBV	62374	72093	1.52%	0.181%
34	16.583	1345	1347	1353	rVB	89665	154772	3.26%	0.388%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052615\
Data File : BF079489.D
Acq On : 26 May 2015 21:52
Operator : TP/IZ
Sample : G2362-03RE
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FK-GF-01-015-BRE

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052615.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	16.971	1378	1381	1384	rBV2	50156	116883	2.46%	0.293%
36	17.040	1384	1387	1390	rVB	255753	307701	6.48%	0.772%
37	17.154	1395	1397	1404	rVV	79901	249095	5.24%	0.625%
38	17.348	1412	1414	1420	rBV3	68510	198558	4.18%	0.498%
39	17.474	1423	1425	1428	rBV2	69566	104158	2.19%	0.261%
40	17.543	1428	1431	1433	rBV	73809	130307	2.74%	0.327%
41	17.600	1433	1436	1439	rBV	1249474	1509001	31.77%	3.785%
42	18.240	1490	1492	1495	rVB	104784	162426	3.42%	0.407%
43	18.617	1523	1525	1531	rVB	104290	202256	4.26%	0.507%


Sum of corrected areas: 39869527

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052615\
Data File : BF079489.D
Acq On : 26 May 2015 21:52
Operator : TP/IZ
Sample : G2362-03RE
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FK-GF-01-015-BRE

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

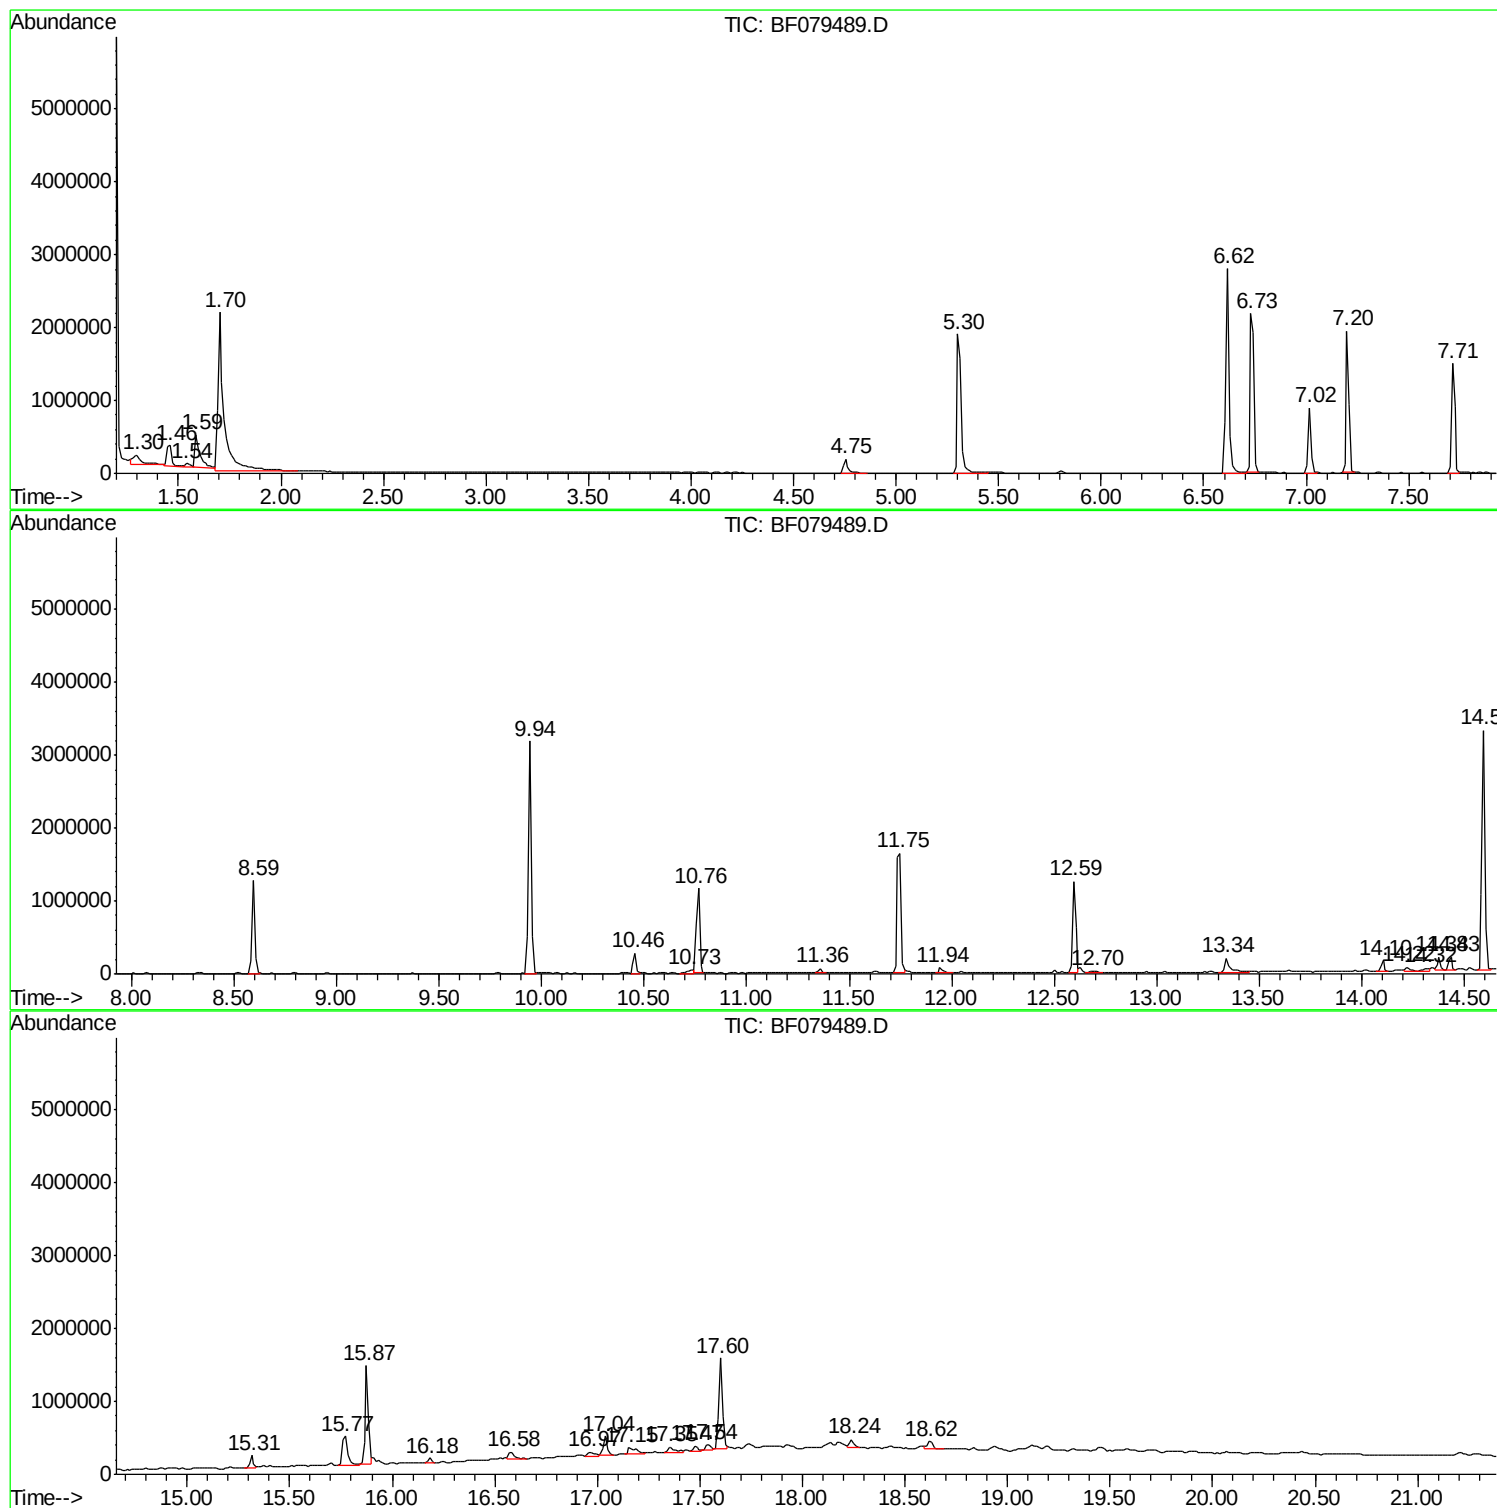

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF052615\
Data_File : BF079489.D
Acq_On : 26 May, 2015 21:522
Operator : TP/IZZ
Sample : G2362-03REE
Misc :
ALS_Vial : 12 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
FK-GF-01-015-BRE

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052615.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION.NN

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
