


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052615\
 Data File : BF079476.D
 Acq On : 26 May 2015 13:43
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052615.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 27 01:32:46 2015

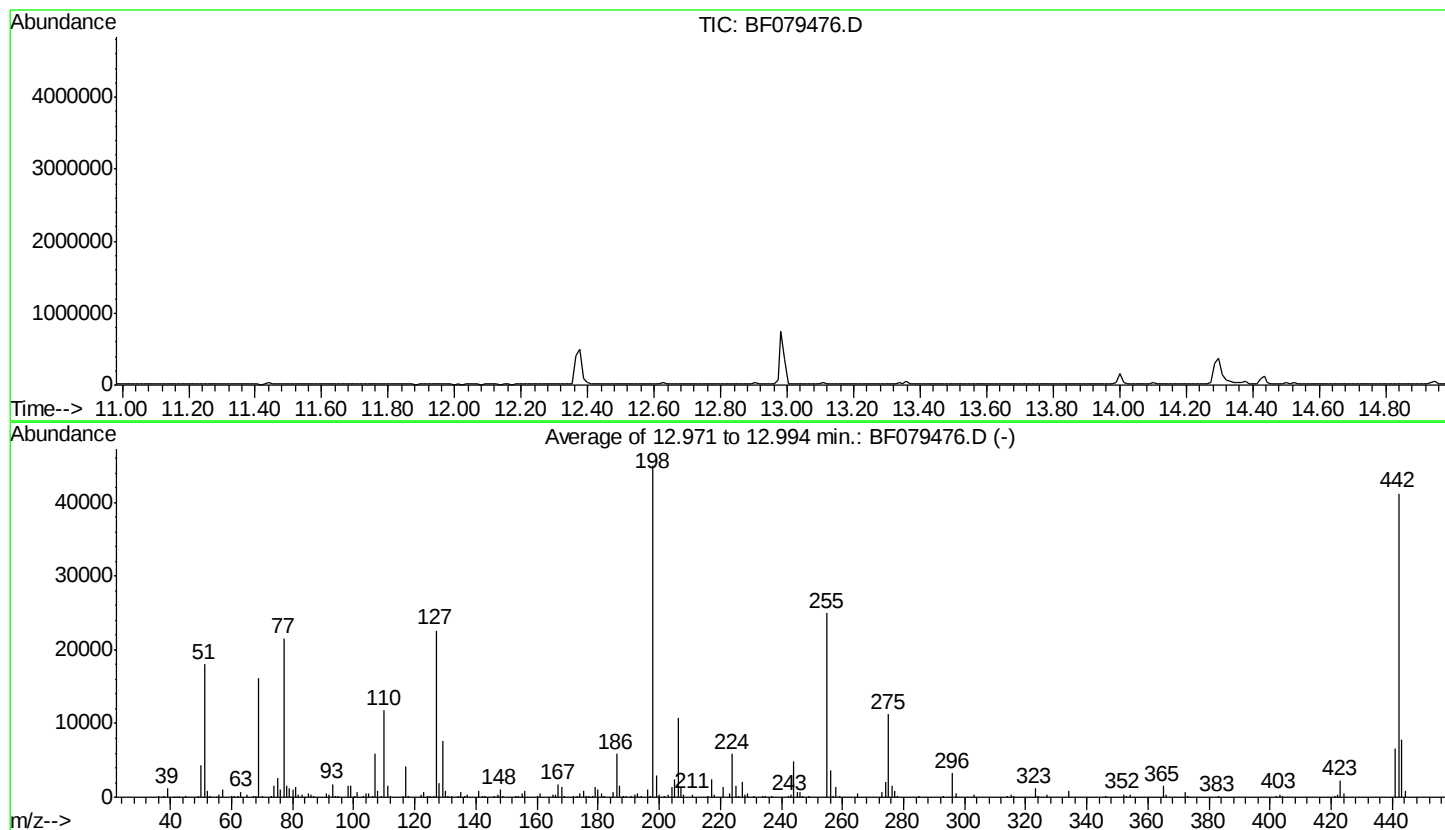

AutoFind: Scans 1031, 1032, 1033; Background Corrected with Scan 1028

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.1	18075	PASS
68	69	0.00	2	1.5	243	PASS
69	198	0.00	100	35.7	16094	PASS
70	69	0.00	2	1.1	172	PASS
127	198	10	80	50.2	22601	PASS
197	198	0.00	2	0.4	183	PASS
198	198	100	100	100.0	45025	PASS
199	198	5	9	6.4	2881	PASS
275	198	10	60	25.0	11239	PASS
365	198	1	100	3.3	1506	PASS
441	442	0.01	24	16.0	6580	PASS
442	198	50	100	91.6	41231	PASS
443	442	15	24	18.9	7809	PASS