


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052615\
 Data File : BF079509.D
 Acq On : 27 May 2015 8:06
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052615.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 27 07:31:10 2015

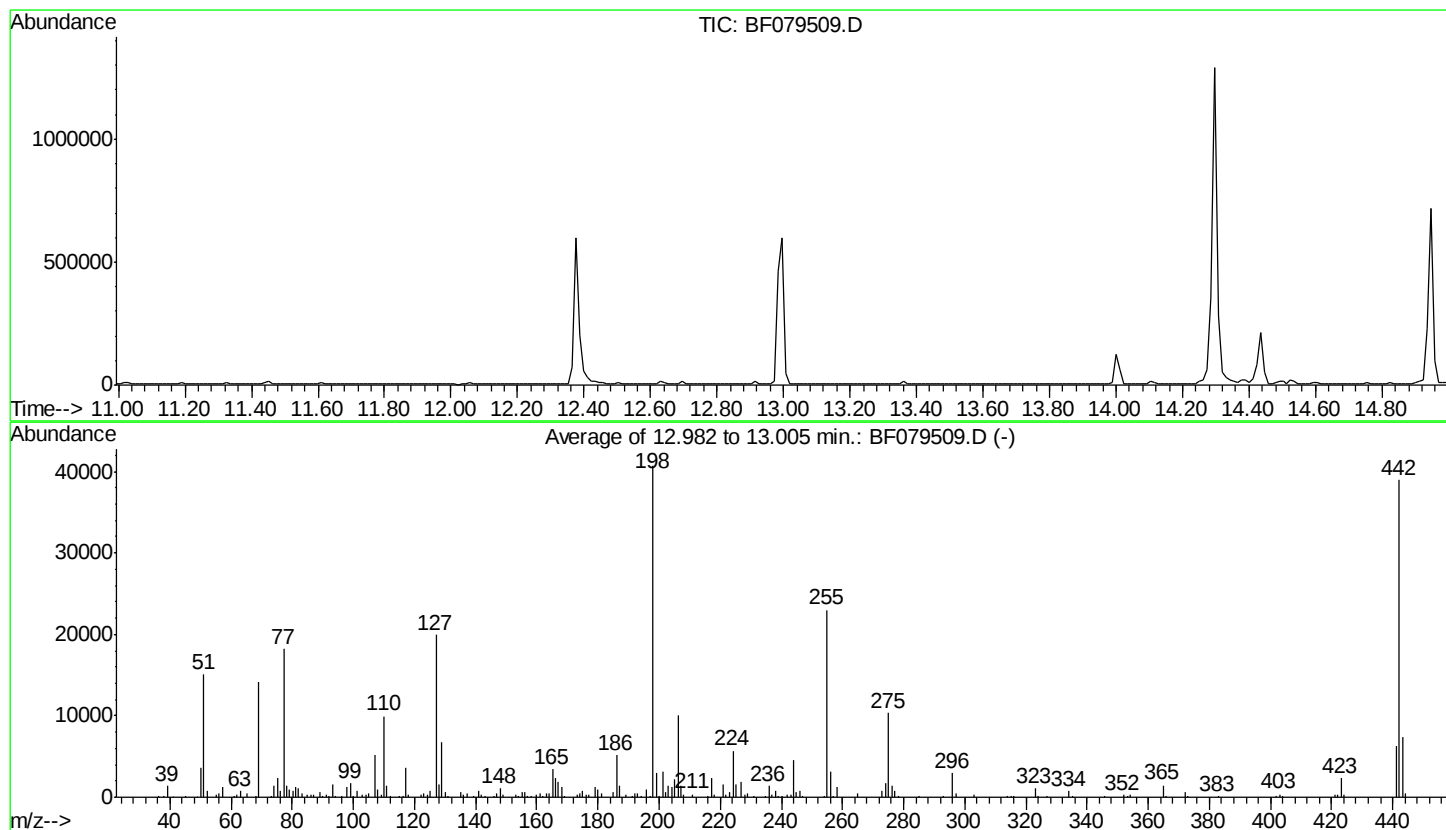

AutoFind: Scans 1032, 1033, 1034; Background Corrected with Scan 1028

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.0	15061	PASS
68	69	0.00	2	1.1	151	PASS
69	198	0.00	100	34.6	14088	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.0	19966	PASS
197	198	0.00	2	0.3	132	PASS
198	198	100	100	100.0	40729	PASS
199	198	5	9	7.3	2987	PASS
275	198	10	60	25.4	10354	PASS
365	198	1	100	3.6	1467	PASS
441	442	0.01	24	16.1	6254	PASS
442	198	50	100	95.6	38955	PASS
443	442	15	24	19.1	7427	PASS