
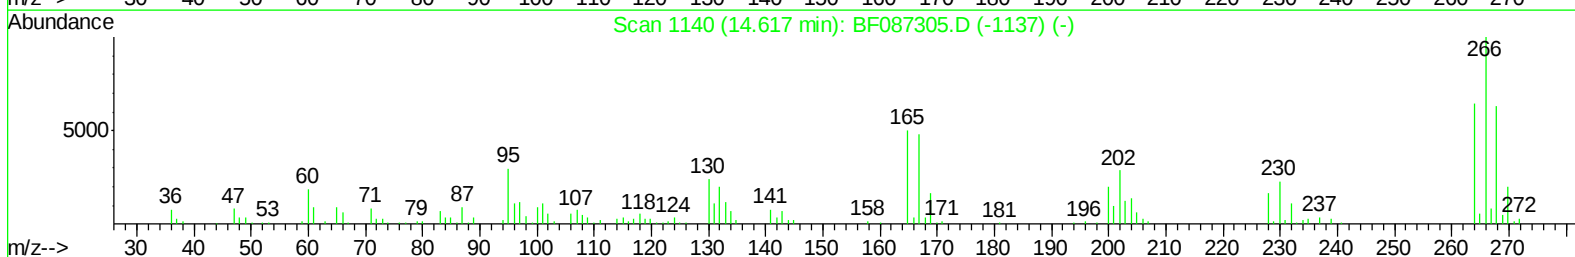
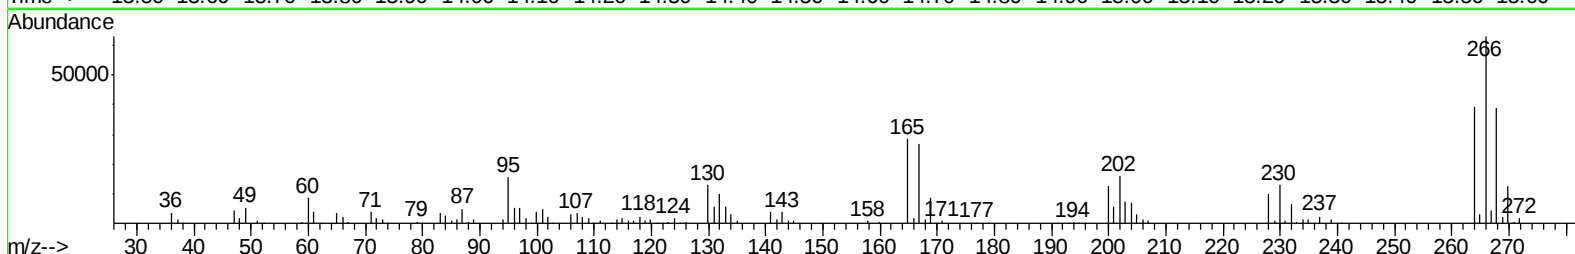


Data Path : Z:\HPCHEM1\BNA F\Data\BF052616\
Data File : BF087407.D
Acq On : 26 May 2016 14:19
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 26 14:45:57 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 25 16:26:52 2016
Response via : Initial Calibration

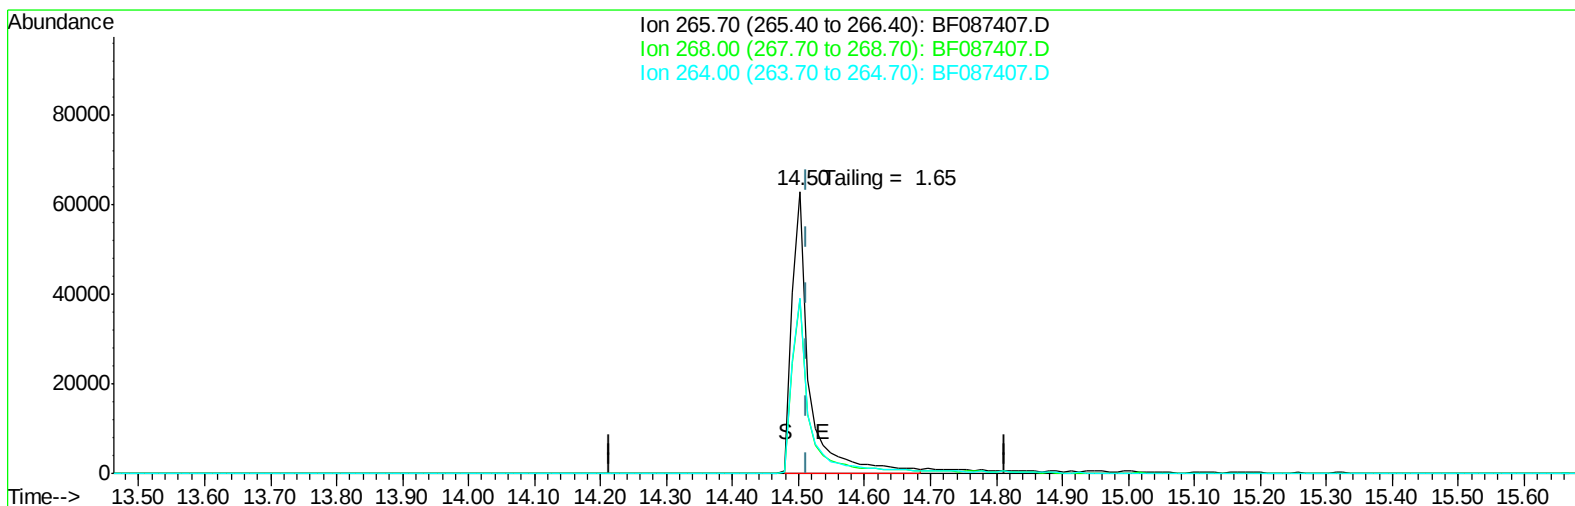

TIC: BF087407.D

(69) Pentachlorophenol (C)




14.502min (-0.011) 0.00ng

response 115133

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	61.60
264.00	66.10	62.42
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF052616\
Data File : BF087407.D
Acq On : 26 May 2016 14:19
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 26 14:45:57 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 25 16:26:52 2016
Response via : Initial Calibration

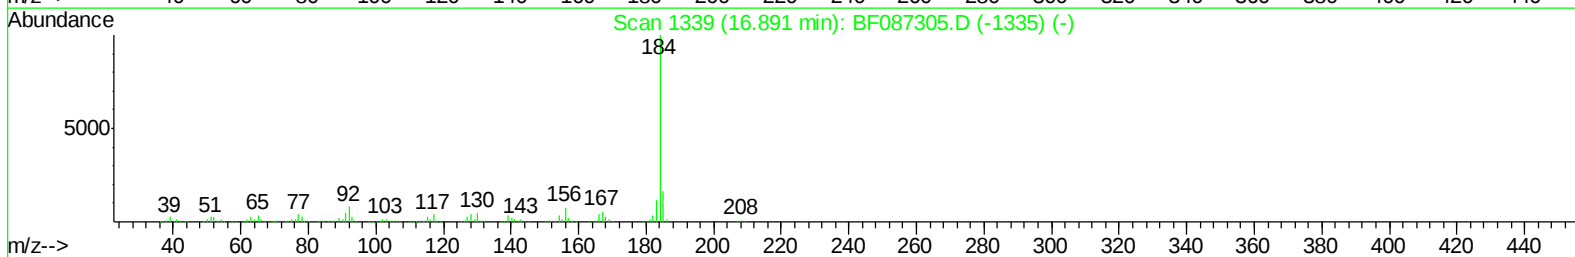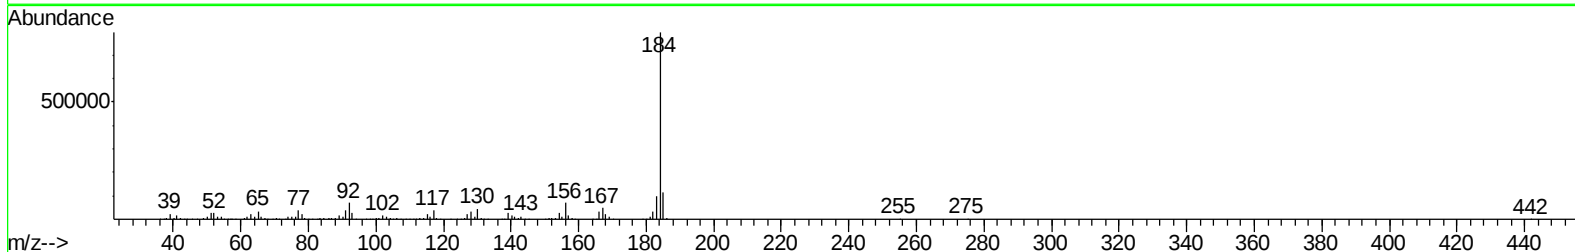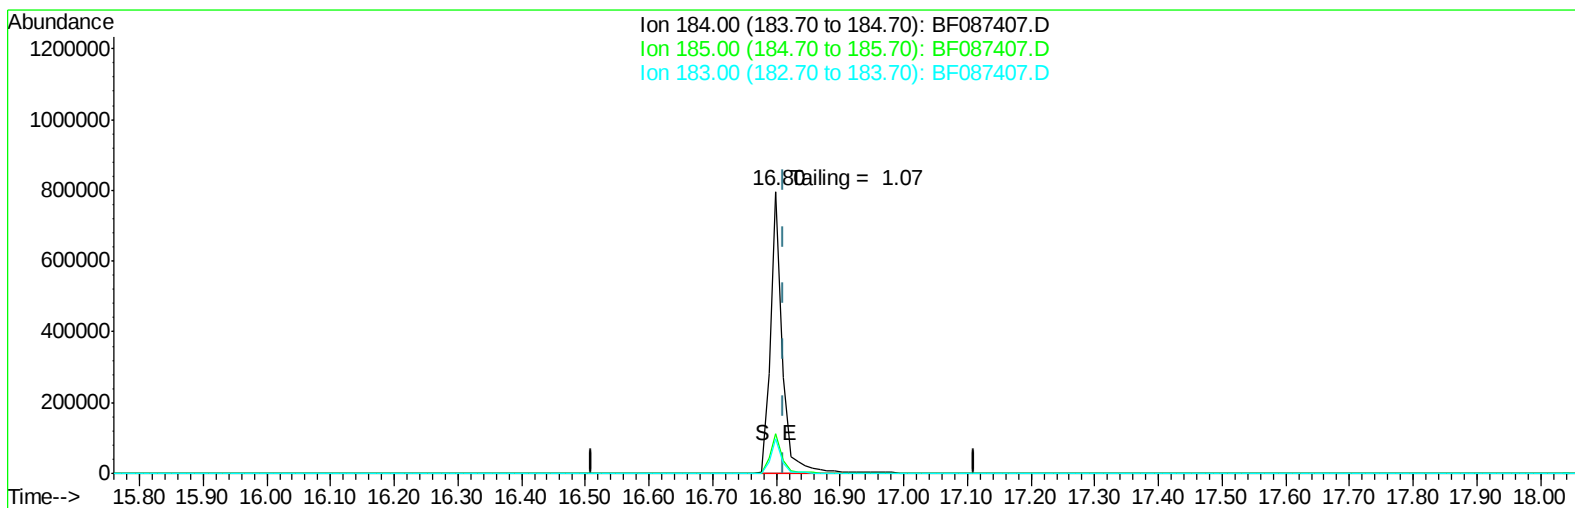

TIC: BF087407.D

(76) Benzidine

16.800min (-0.011) 0.00ng

response 1052257

Ion	Exp%	Act%
184.00	100	100
185.00	17.00	14.32
183.00	12.20	12.30
0.00	0.00	0.00