
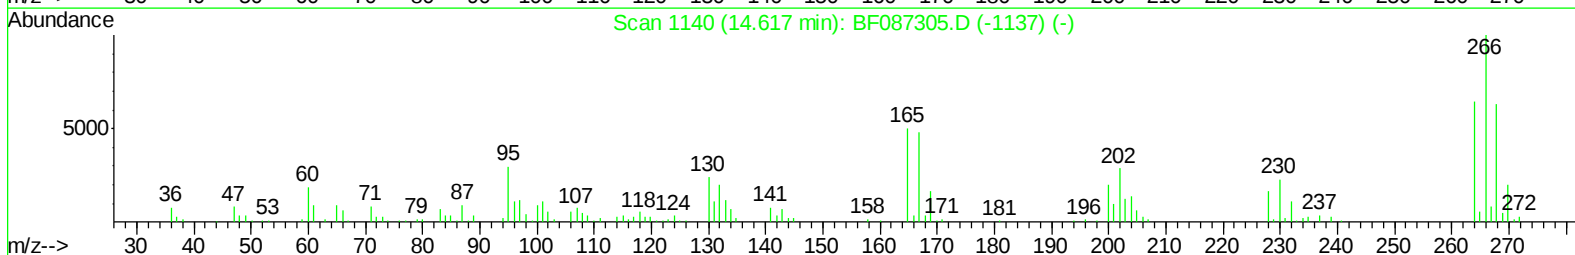
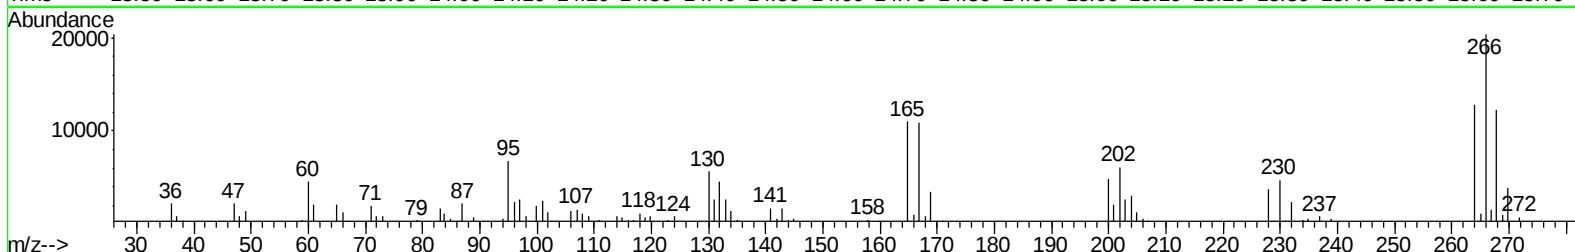


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052616\
Data File : BF087429.D
Acq On : 27 May 2016 3:47
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 27 04:14:28 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 25 16:26:52 2016
Response via : Initial Calibration

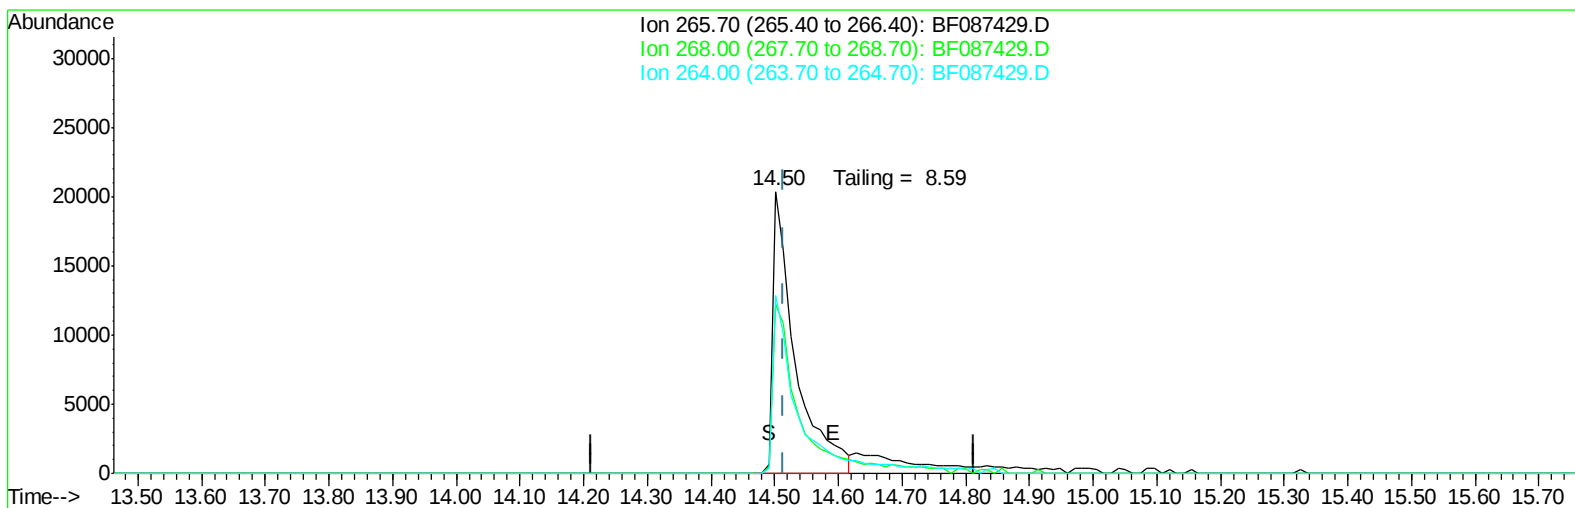

TIC: BF087429.D

(69) Pentachlorophenol (C)




14.502min (-0.011) 0.00ng

response 57790

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	60.07
264.00	66.10	63.00
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052616\
 Data File : BF087429.D
 Acq On : 27 May 2016 3:47
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 27 04:14:28 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 25 16:26:52 2016
 Response via : Initial Calibration

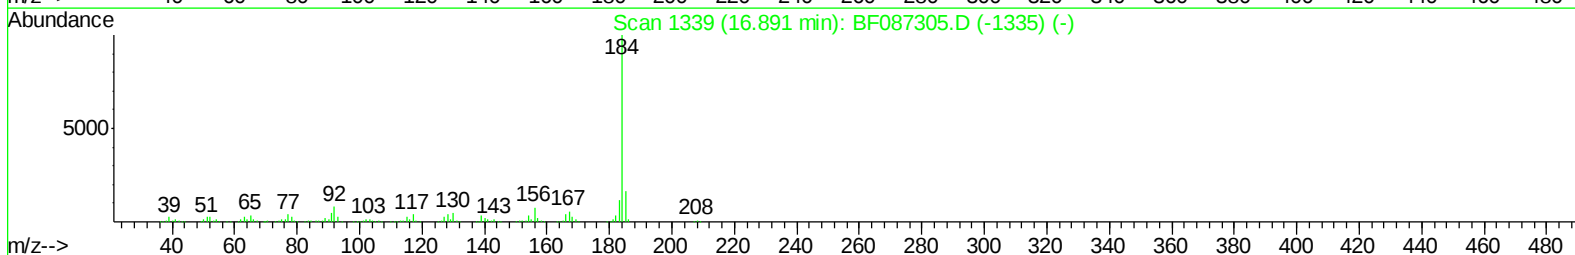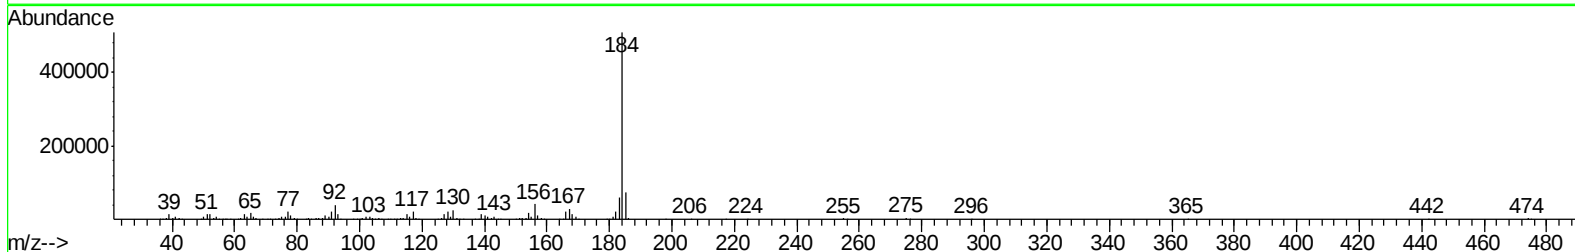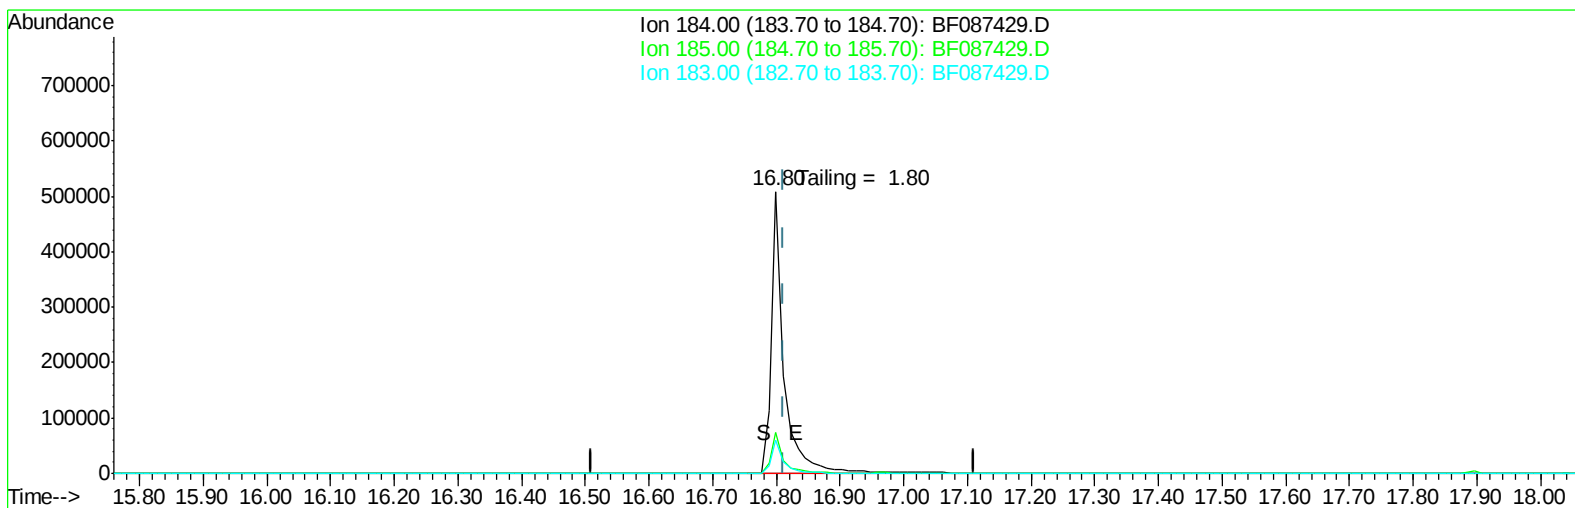

TIC: BF087429.D

(76) Benzidine

16.800min (-0.011) 0.00ng

response 712306

Ion	Exp%	Act%
184.00	100	100
185.00	17.00	14.40
183.00	12.20	12.02
0.00	0.00	0.00