


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052616\
 Data File : BF087407.D
 Acq On : 26 May 2016 14:19
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 27 17:03:59 2016

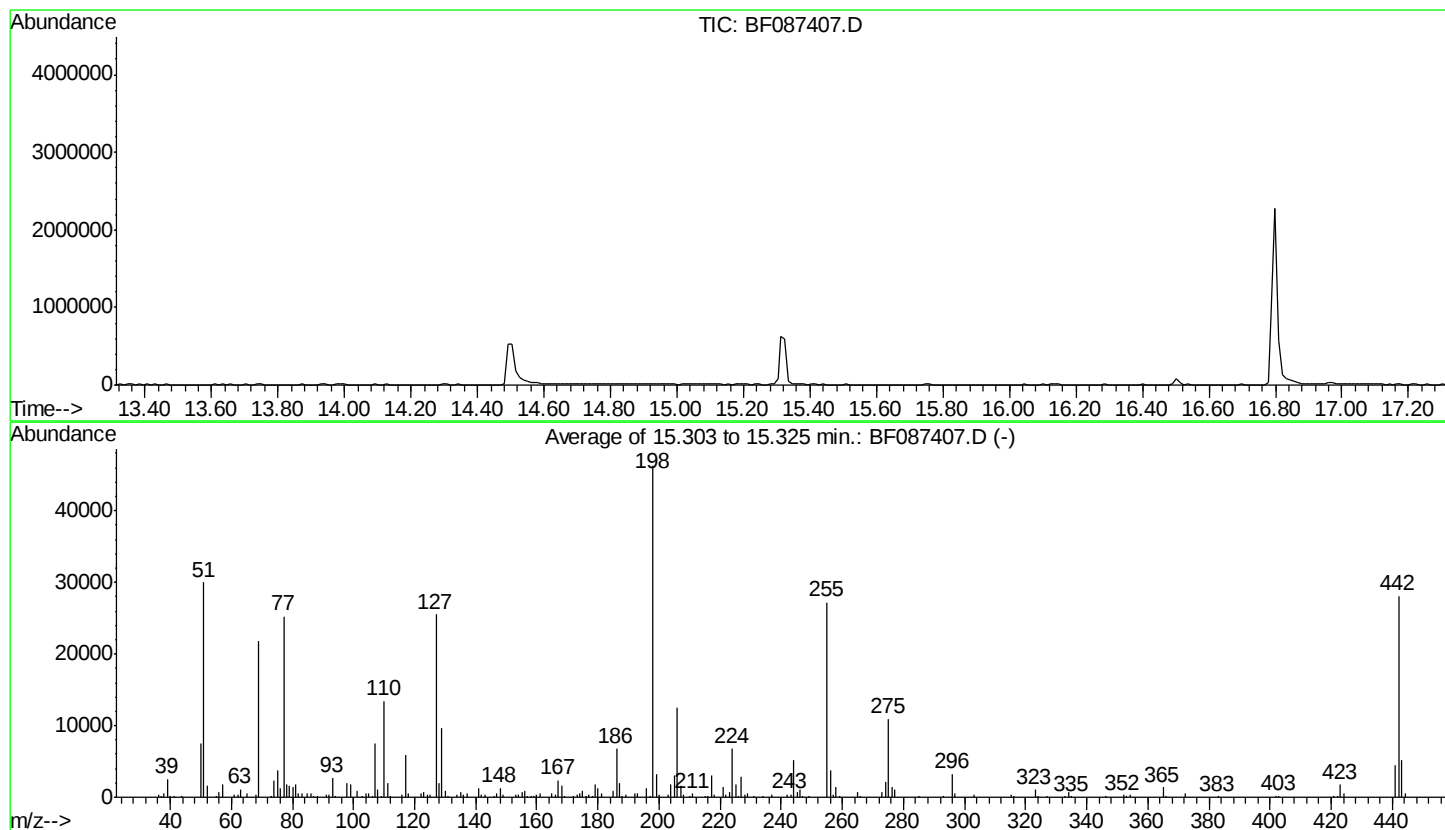

AutoFind: Scans 1200, 1201, 1202; Background Corrected with Scan 1197

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	64.7	29951	PASS
68	69	0.00	2	1.8	393	PASS
69	198	0.00	100	47.2	21853	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	55.0	25486	PASS
197	198	0.00	2	0.4	177	PASS
198	198	100	100	100.0	46306	PASS
199	198	5	9	6.8	3139	PASS
275	198	10	60	23.6	10907	PASS
365	198	1	100	3.1	1430	PASS
441	442	0.01	24	16.2	4547	PASS
442	198	50	100	60.7	28123	PASS
443	442	15	24	18.6	5237	PASS