
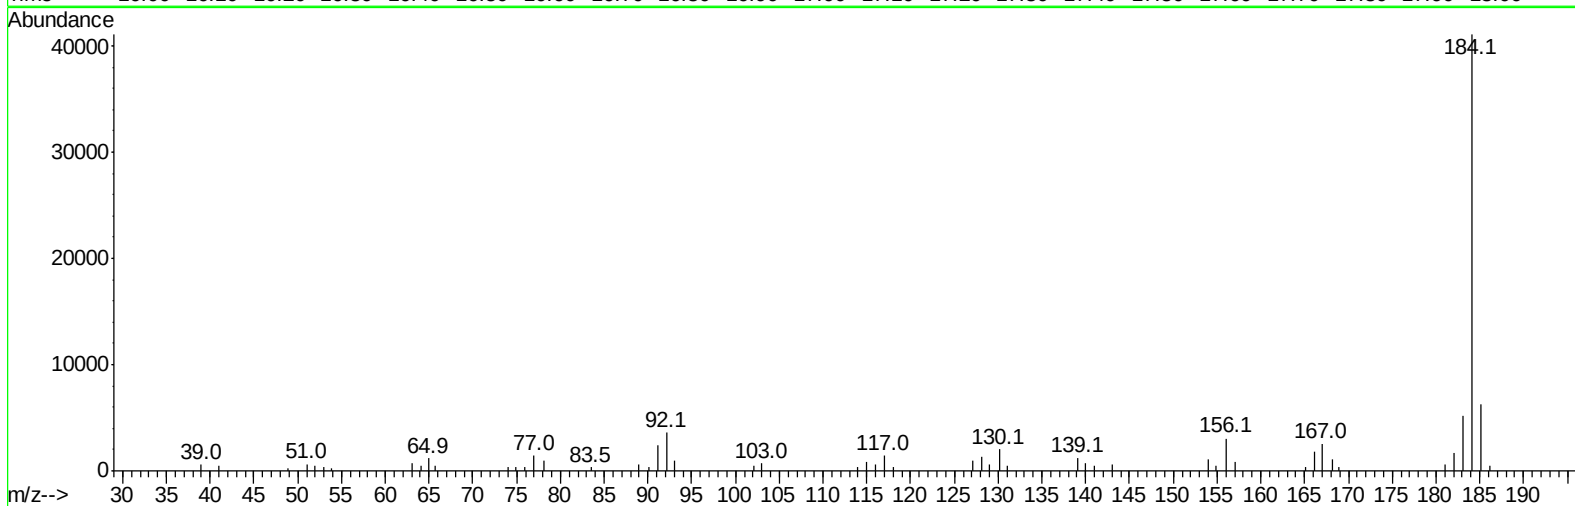


Data Path : Z:\HPCHEM1\BNA F\DATA\BF052617\
Data File : BF095477.D
Acq On : 27 May 2017 00:59
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 29 00:27:59 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 26 16:50:16 2017
Response via : Initial Calibration

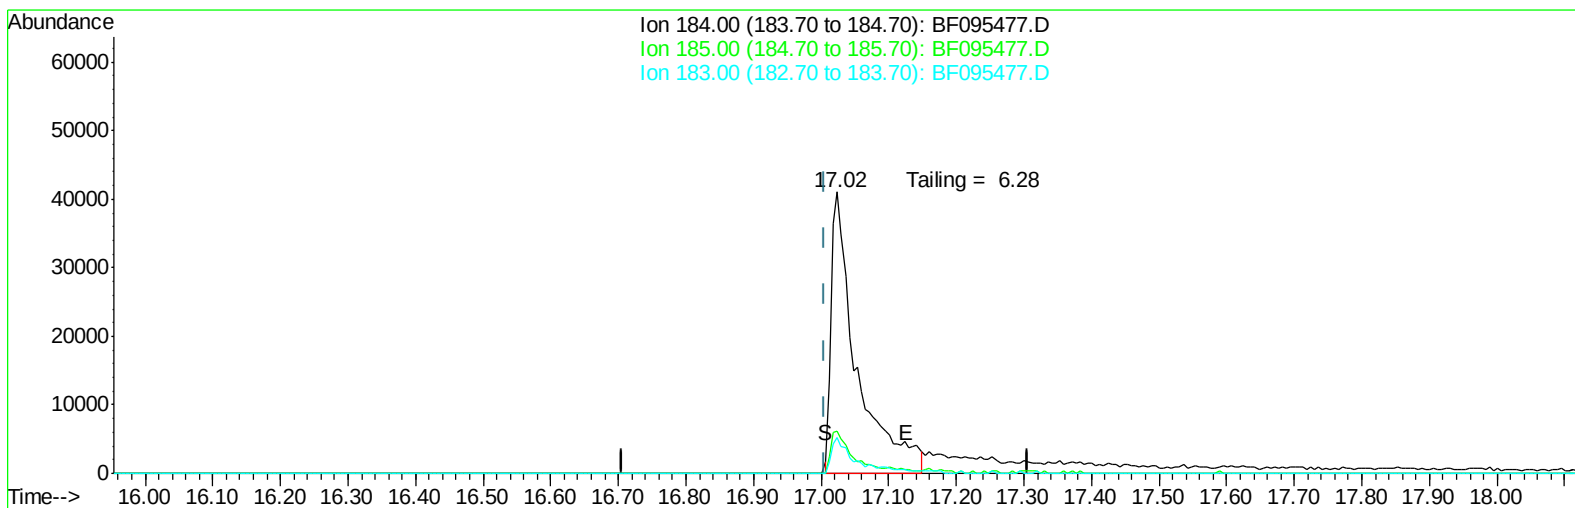

TIC: BF095477.D

(76) Benzidine



17.024min (+0.018) 1953.95ng

response 100300

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	15.19#
183.00	12.20	12.67
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF052617\
Data File : BF095477.D
Acq On : 27 May 2017 00:59
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 29 00:27:59 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 26 16:50:16 2017
Response via : Initial Calibration

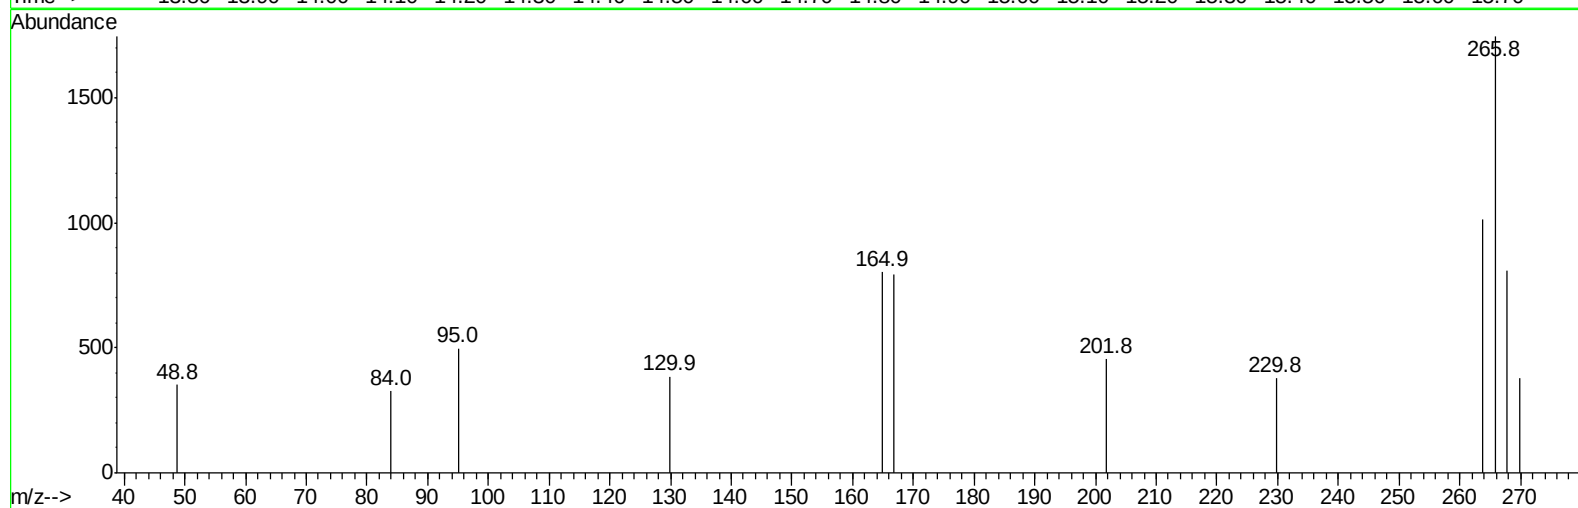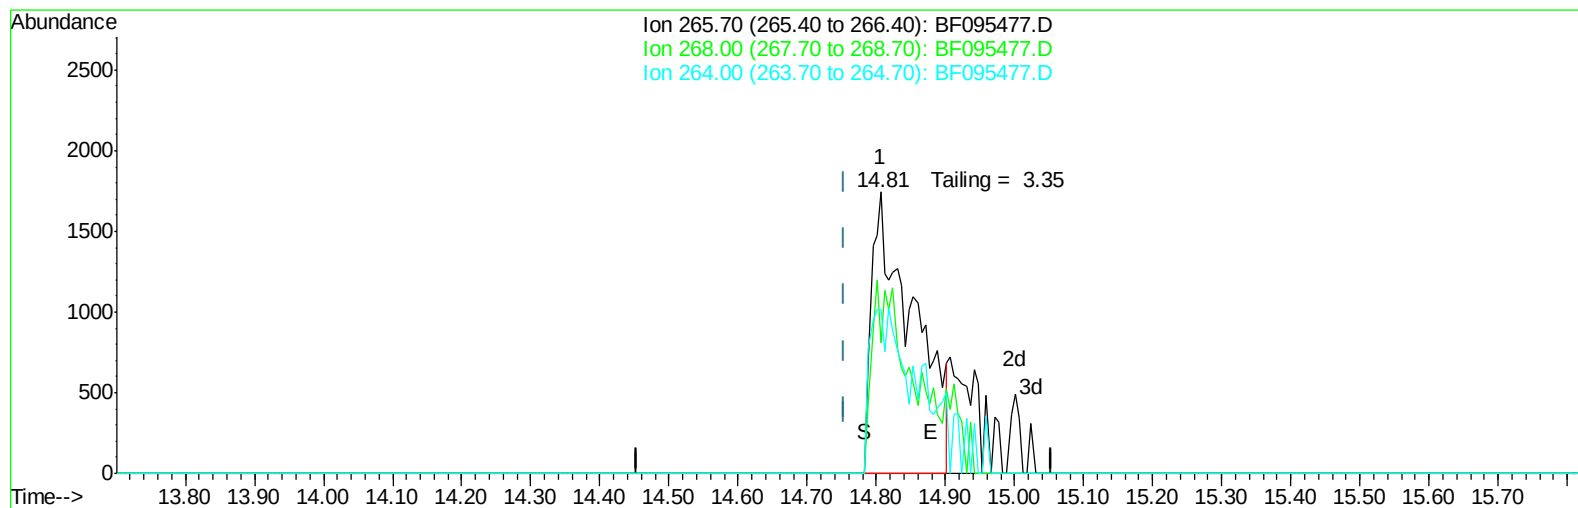

TIC: BF095477.D

(69) Pentachlorophenol (C)

14.807min (+0.053) 0.00ng

response 2740

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	46.25#
264.00	64.60	57.99
0.00	0.00	0.00