

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052617\
 Data File : BF095492.D
 Acq On : 27 May 2017 9:15
 Operator : SJ/MA
 Sample : I3239-01 1000X
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PURGE-WATER-A

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	7.766	988	991	1007	rBV	90276	285065	58.71%	12.282%
2	9.783	1329	1334	1355	rBV	138161	437831	90.18%	18.863%
3	12.613	1810	1815	1826	rBV2	217090	485531	100.00%	20.919%
4	12.760	1838	1840	1850	rVB3	4134	6999	1.44%	0.302%
5	15.018	2219	2224	2242	rBV	142301	351442	72.38%	15.141%
6	18.683	2843	2847	2865	rBV	199371	377541	77.76%	16.266%
7	20.071	3078	3083	3084	rBV3	5612	6601	1.36%	0.284%
8	20.365	3128	3133	3154	rBV	149206	318863	65.67%	13.738%
9	20.794	3204	3206	3210	rVB4	8321	9028	1.86%	0.389%
10	21.224	3275	3279	3284	rBV6	6243	10325	2.13%	0.445%
11	21.724	3360	3364	3369	rVB6	9232	20678	4.26%	0.891%
12	21.800	3369	3377	3379	rBV8	5567	11150	2.30%	0.480%


Sum of corrected areas: 2321054

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052617\
Data File : BF095492.D
Acq On : 27 May 2017 9:15
Operator : SJ/MA
Sample : I3239-01 1000X
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PURGE-WATER-A

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

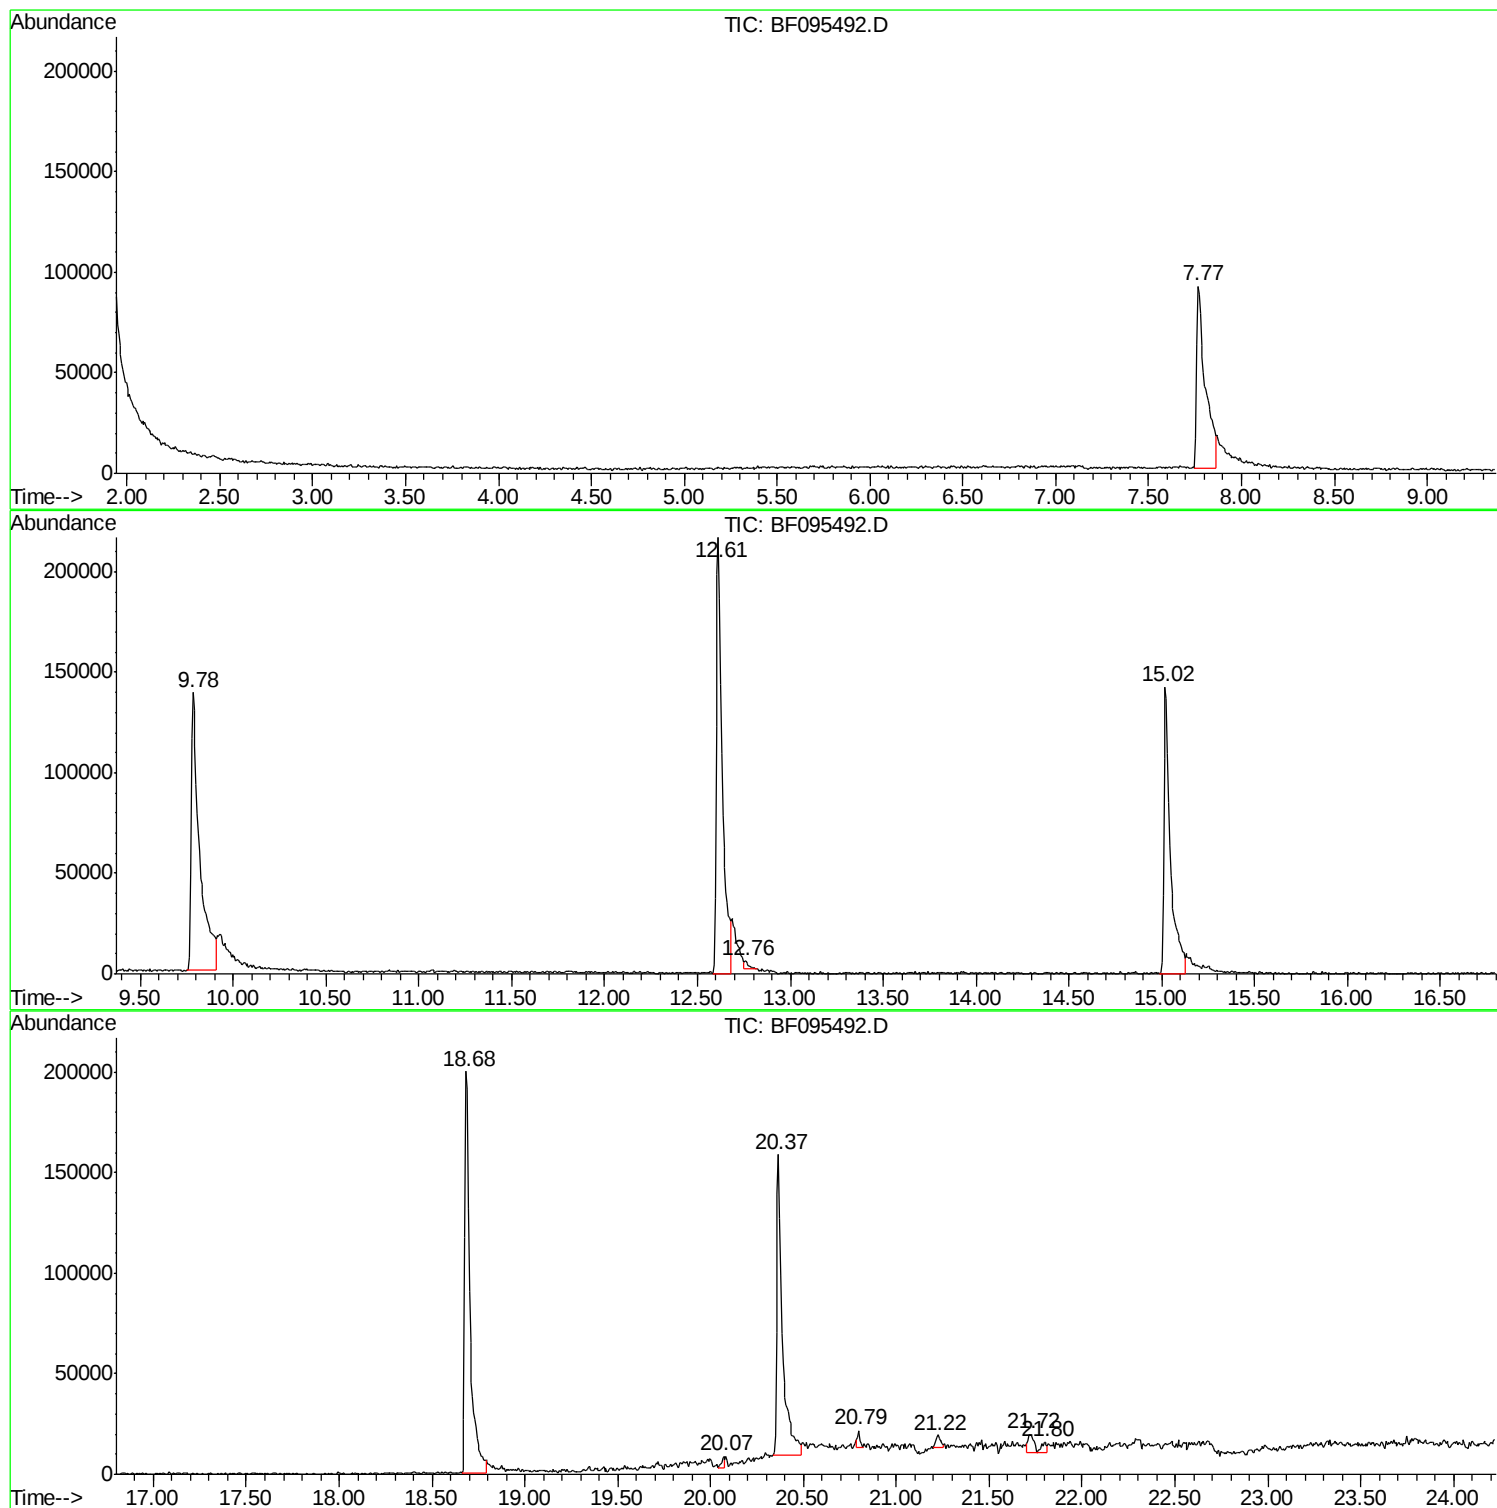

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF052617\
Data_File : BF095492.D
Acq_On : 22 May, 2017 9:155
Operator : SJ/MAA
Sample : I3239-01_1000XX
Misc :
ALS_Vial : 37 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
PURGE-WATER-A

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION.NN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
