


Data Path : Z:\HPCHEM1\BNA F\Data\BF052617\
 Data File : BF095454.D
 Acq On : 26 May 2017 11:29
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 26 16:50:16 2017

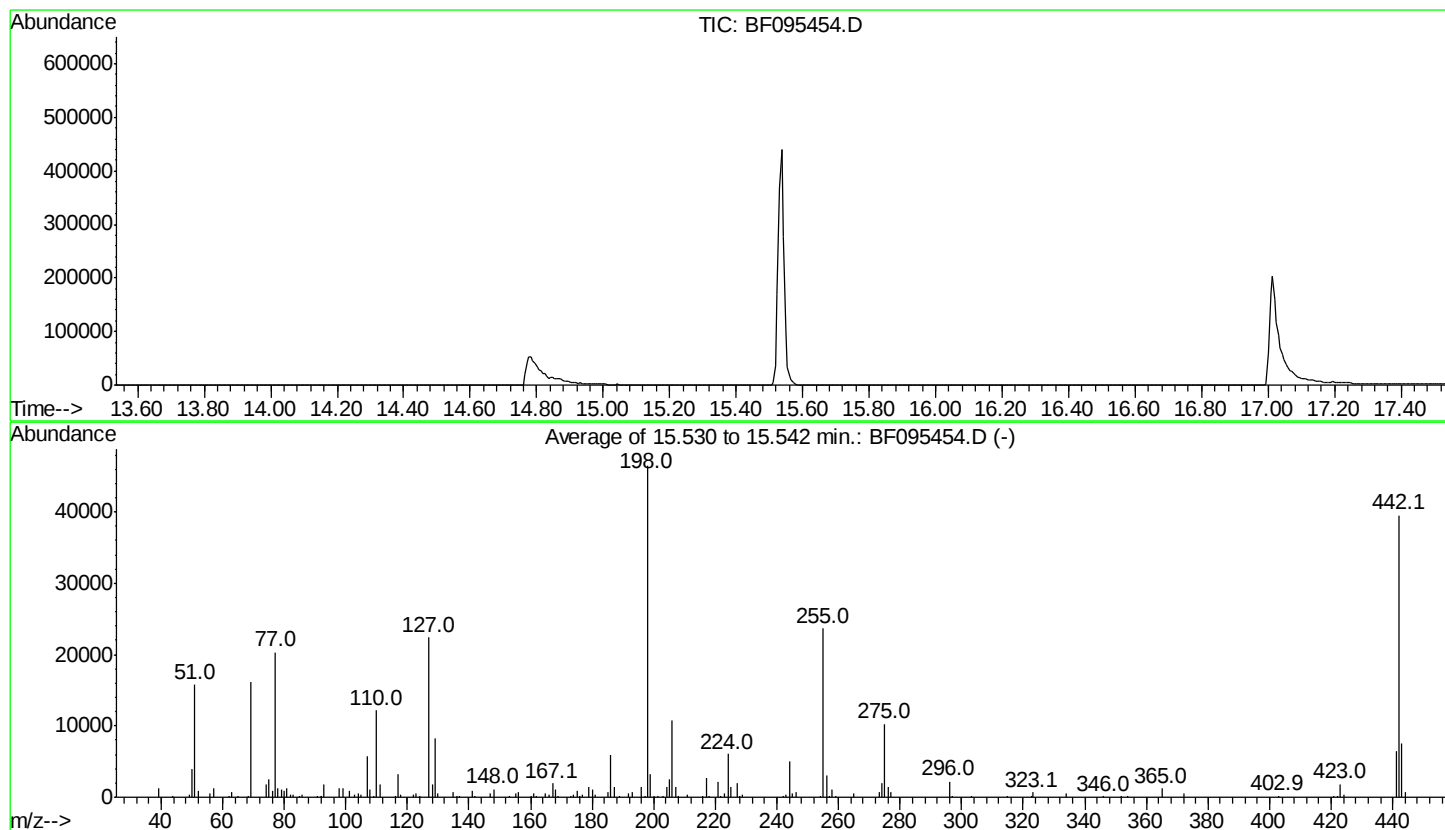

AutoFind: Scans 2311, 2312, 2313; Background Corrected with Scan 2305

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.8	15730	PASS
68	69	0.00	2	0.9	139	PASS
69	198	0.00	100	34.9	16234	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.1	22369	PASS
197	198	0.00	2	0.3	145	PASS
198	198	100	100	100.0	46488	PASS
199	198	5	9	6.9	3185	PASS
275	198	10	60	22.2	10308	PASS
365	198	1	100	2.5	1176	PASS
441	442	0.01	24	16.3	6453	PASS
442	198	50	100	85.1	39562	PASS
443	442	15	24	18.9	7477	PASS