


Data Path : Z:\HPCHEM1\BNA F\Data\BF052617\
Data File : BF095477.D
Acq On : 27 May 2017 00:59
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri May 26 16:50:16 2017

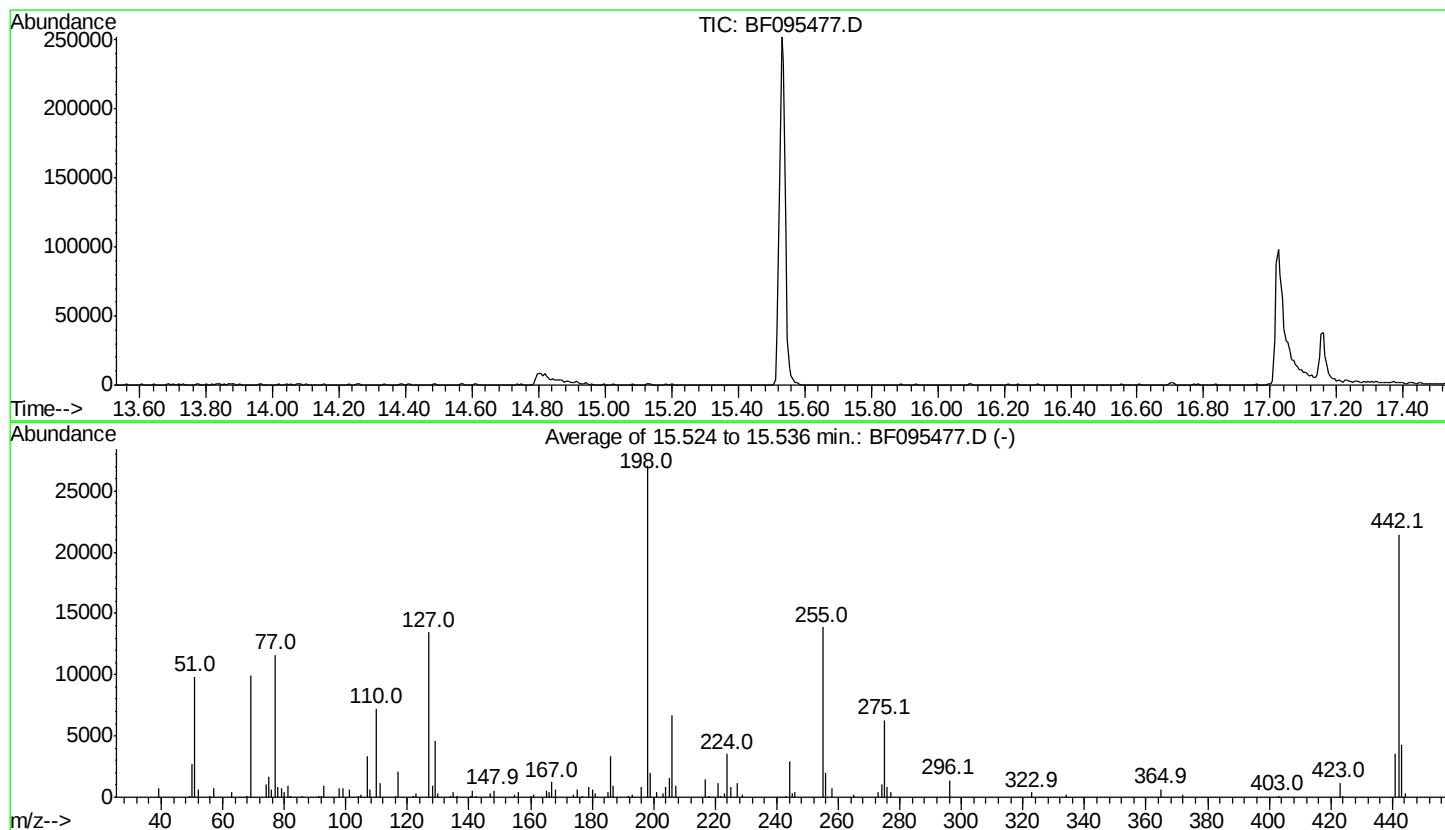

AutoFind: Scans 2310, 2311, 2312; Background Corrected with Scan 2305

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.3	9828	PASS
68	69	0.00	2	1.2	115	PASS
69	198	0.00	100	36.6	9917	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.8	13466	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	27061	PASS
199	198	5	9	7.4	1998	PASS
275	198	10	60	23.2	6270	PASS
365	198	1	100	2.4	643	PASS
441	442	0.01	24	16.8	3606	PASS
442	198	50	100	79.3	21459	PASS
443	442	15	24	19.9	4265	PASS