
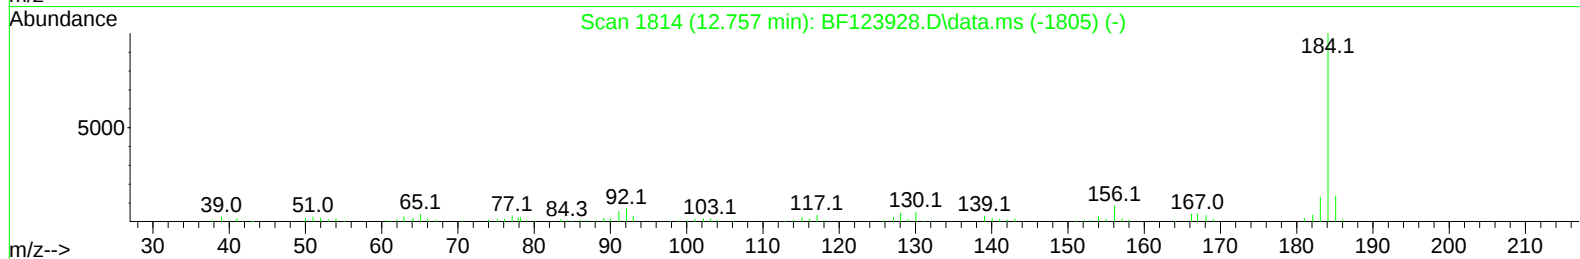
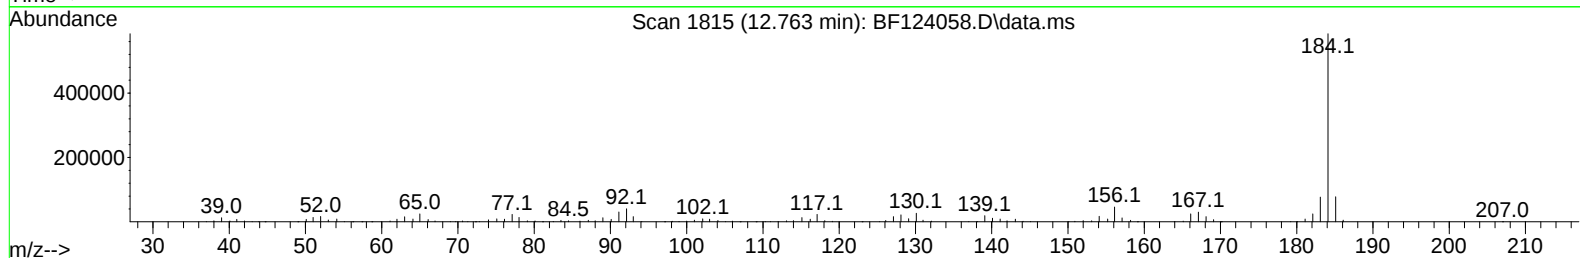


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052621\
Data File : BF124058.D
Acq On : 26 May 2021 10:12
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 26 11:03:30 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 19:05:57 2021
Response via : Initial Calibration

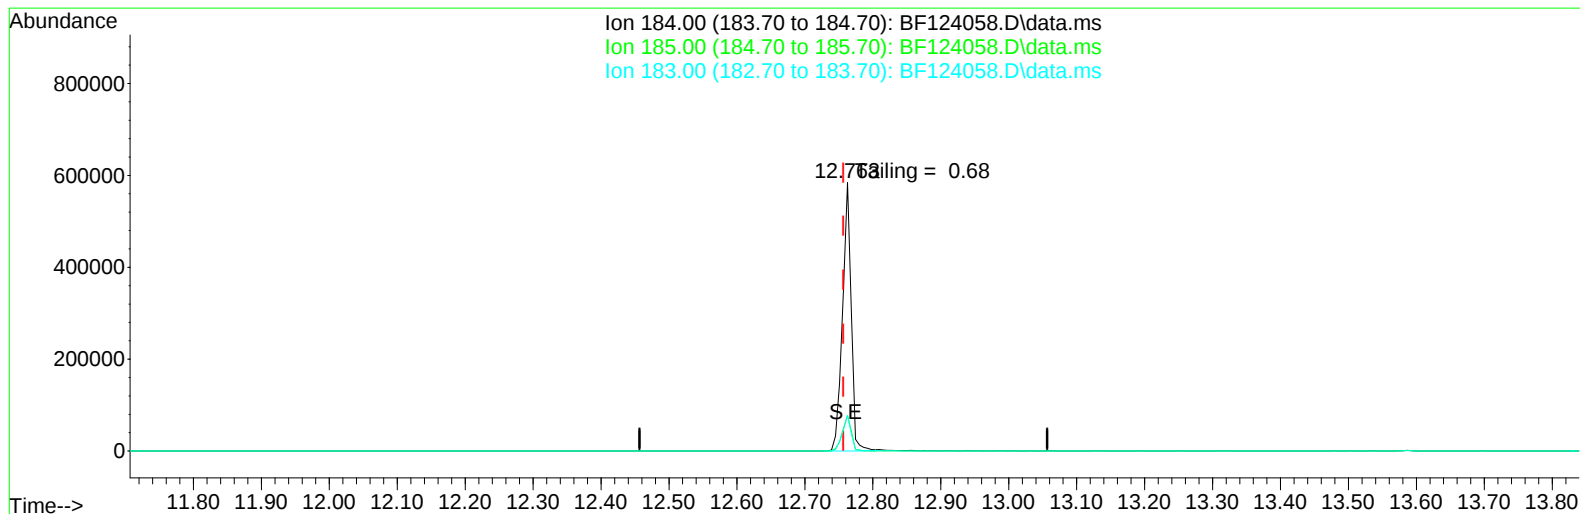

TIC: BF124058.D\data.ms

(77) Benzidine




12.763min (+ 0.006) 0.00 ng

response 523072

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.32
183.00	9.80	13.18#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052621\
Data File : BF124058.D
Acq On : 26 May 2021 10:12
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 26 11:03:30 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 19:05:57 2021
Response via : Initial Calibration

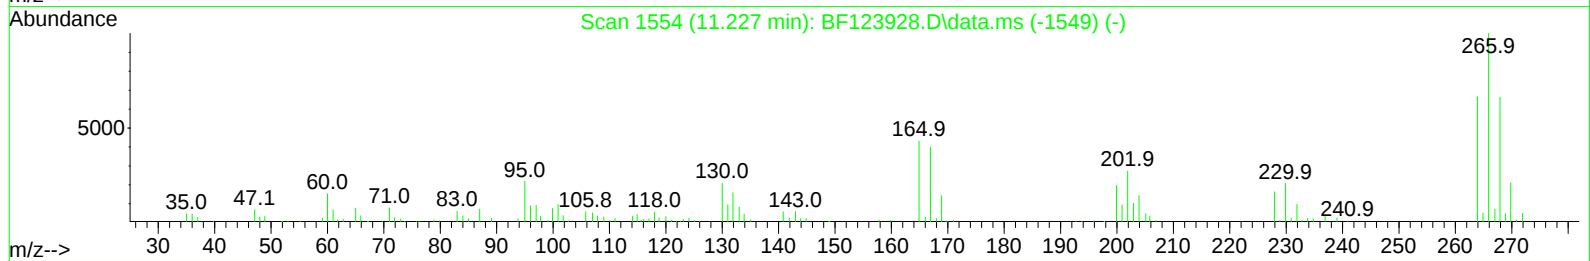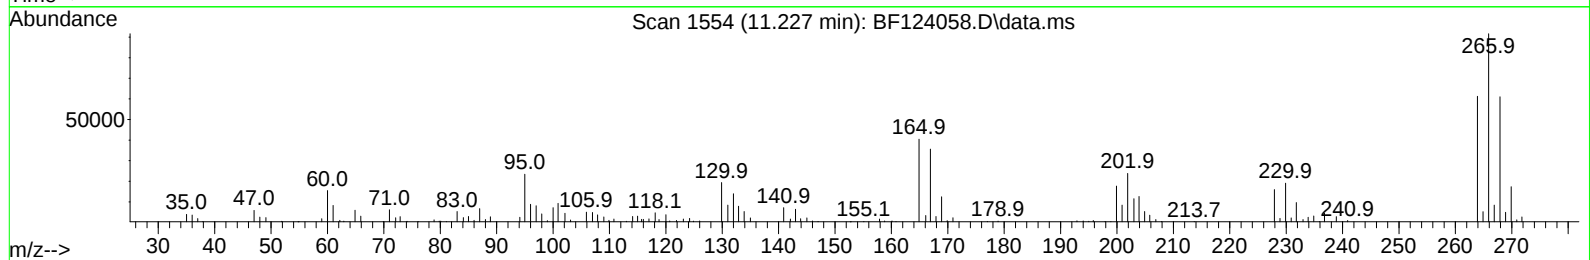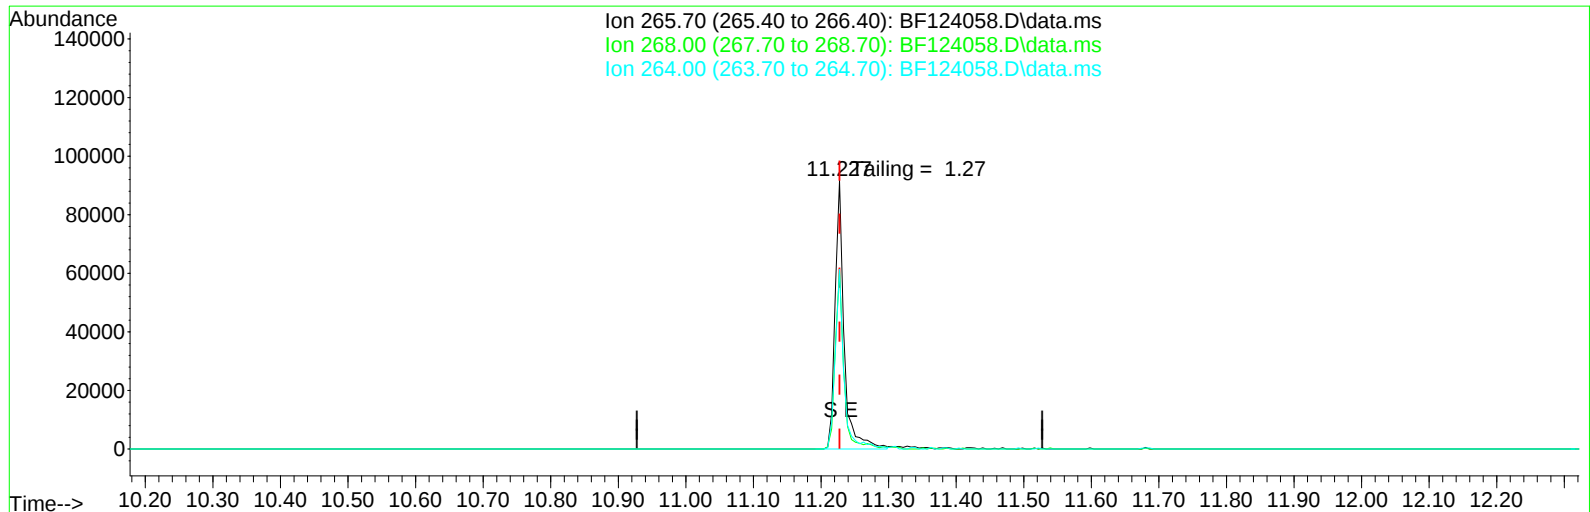

TIC: BF124058.D\data.ms

(70) Pentachlorophenol (C)

11.227min (+ 0.000) 17378.70 ng

response 87370

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	66.57
264.00	65.70	66.88
0.00	0.00	0.00