
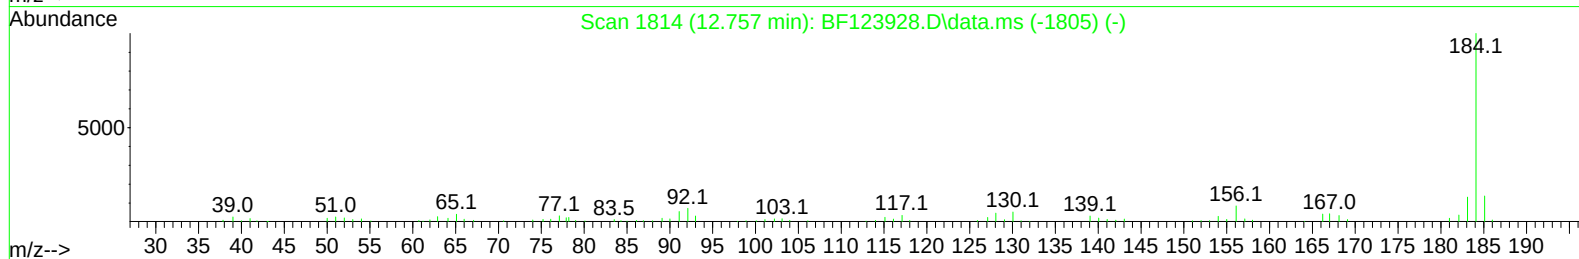
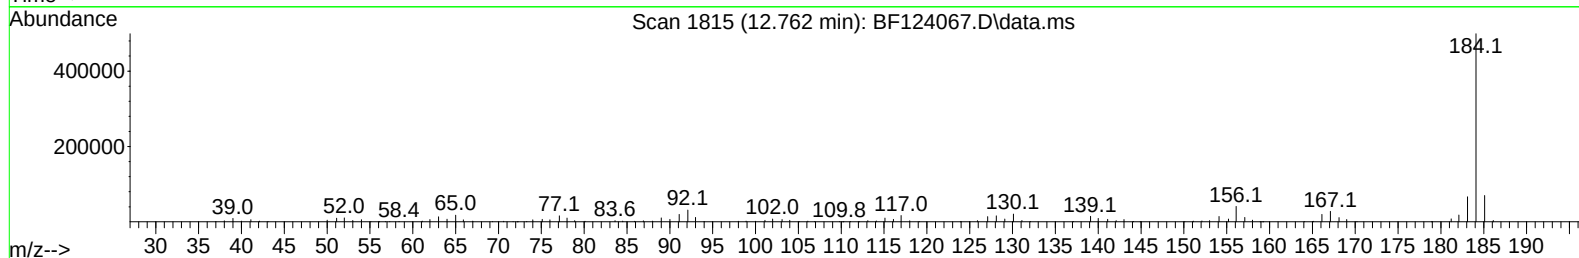


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052621\
 Data File : BF124067.D
 Acq On : 26 May 2021 16:26
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 26 16:53:49 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 14 19:05:57 2021
 Response via : Initial Calibration

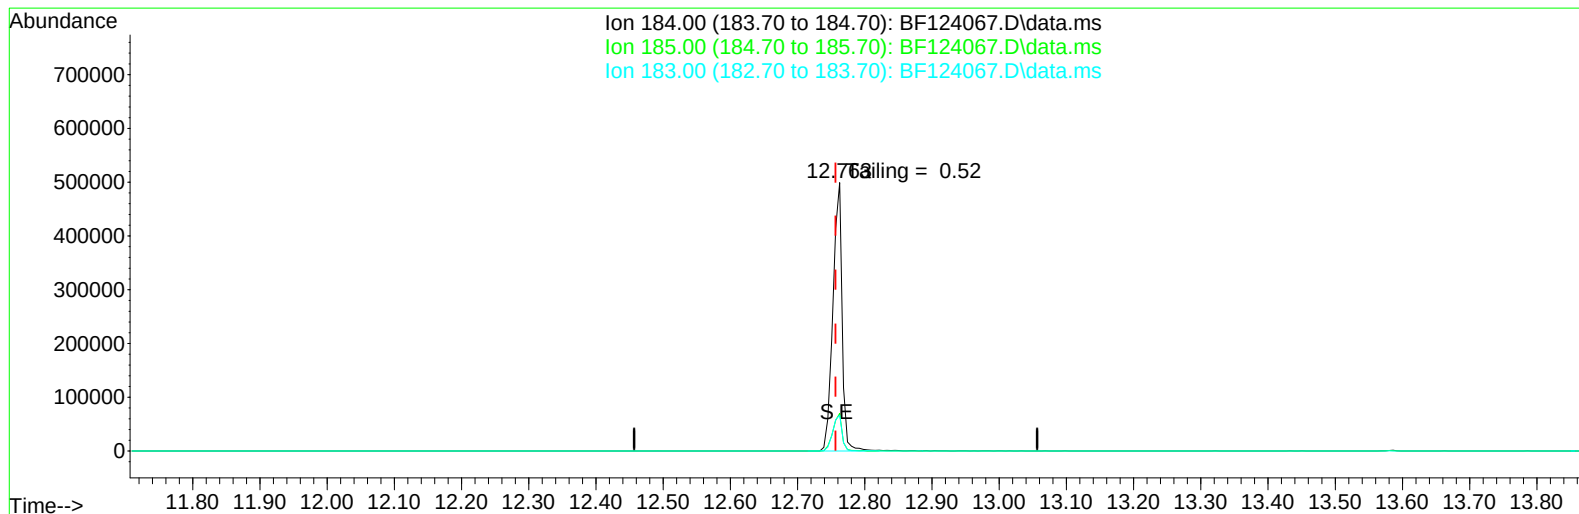

TIC: BF124067.D\data.ms

(77) Benzidine




12.762min (+ 0.006) 0.00 ng

response 478699

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.03
183.00	9.80	13.35#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052621\
Data File : BF124067.D
Acq On : 26 May 2021 16:26
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 26 16:53:49 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 19:05:57 2021
Response via : Initial Calibration

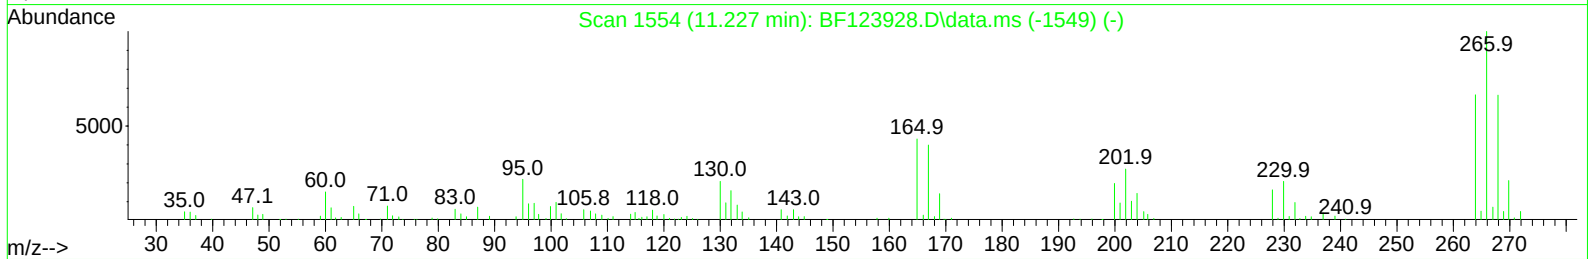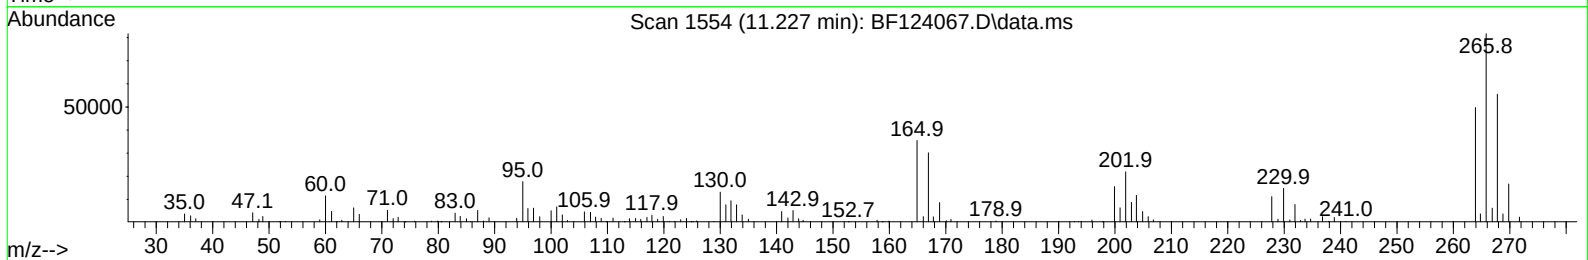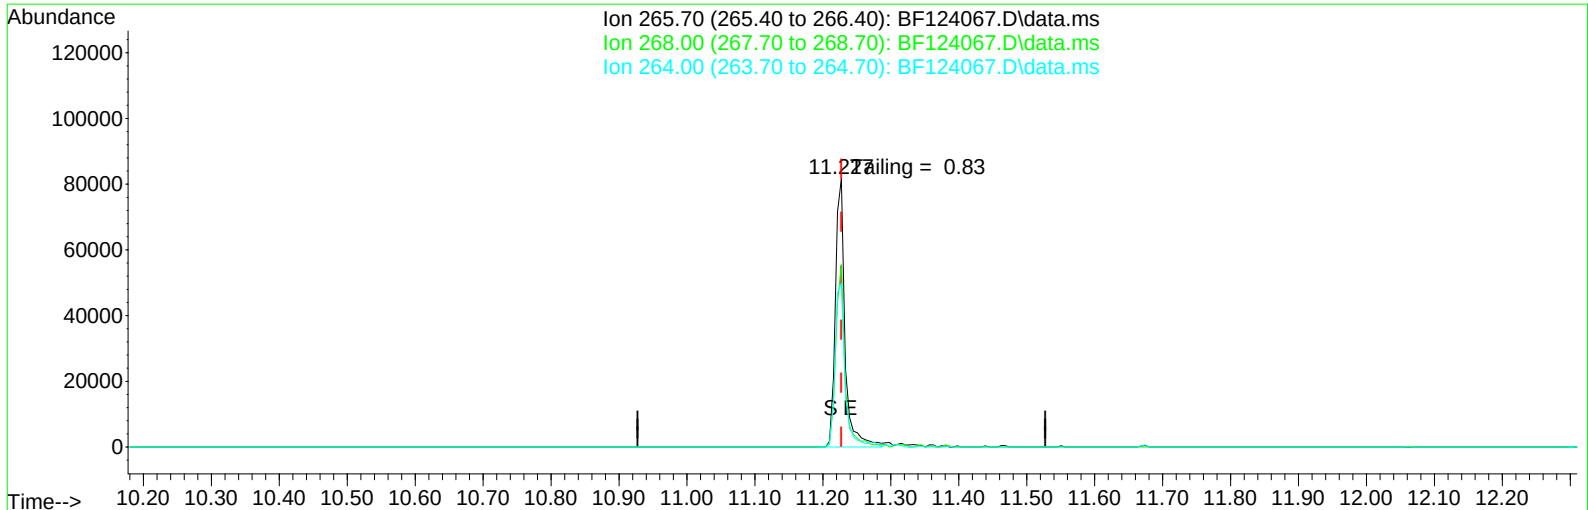

TIC: BF124067.D\data.ms

(70) Pentachlorophenol (C)

11.227min (-0.000) 21245.08 ng

response 82231

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	67.92
264.00	65.70	60.96
0.00	0.00	0.00