
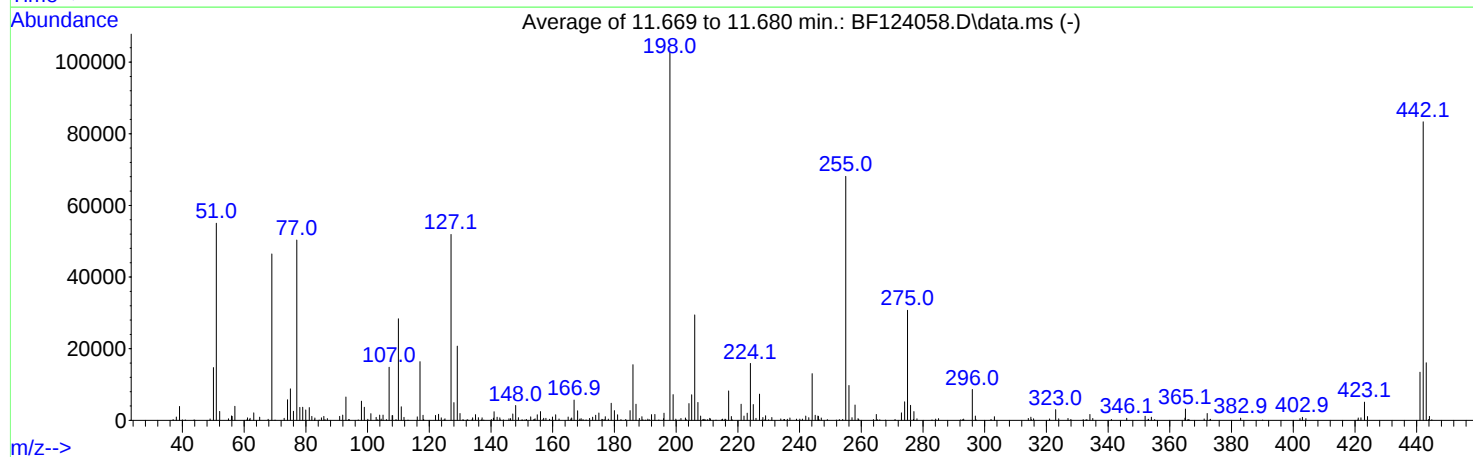


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF052621\  
 Data File : BF124058.D  
 Acq On : 26 May 2021 10:12  
 Operator : JU/CG  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF051421.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu May 27 13:12:25 2021

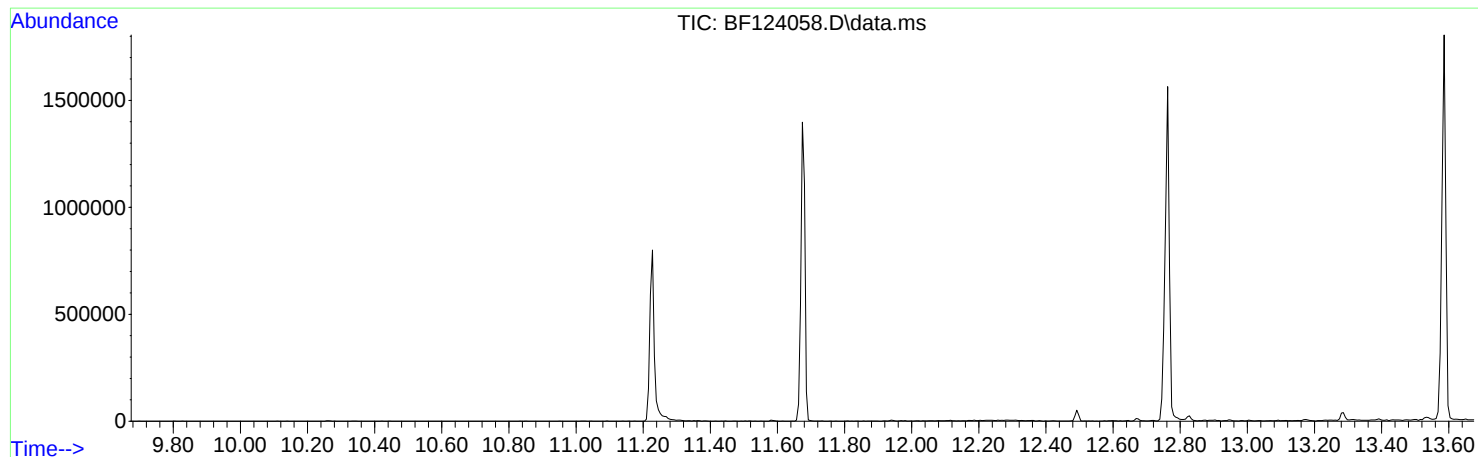




AutoFind: Scans 1629, 1630, 1631; Background Corrected with Scan 1624

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 53.6         | 55005      | PASS                |
| 68             | 69              | 0.00            | 2               | 0.7          | 328        | PASS                |
| 69             | 198             | 0.00            | 100             | 45.2         | 46429      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.2          | 100        | PASS                |
| 127            | 198             | 10              | 80              | 50.5         | 51904      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 102680     | PASS                |
| 199            | 198             | 5               | 9               | 7.0          | 7199       | PASS                |
| 275            | 198             | 10              | 60              | 29.9         | 30747      | PASS                |
| 365            | 198             | 1               | 100             | 3.1          | 3175       | PASS                |
| 441            | 198             | 0.01            | 100             | 13.1         | 13465      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 83320      | PASS                |
| 443            | 442             | 15              | 24              | 19.3         | 16073      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF052621\  
Data File : BF124058.D  
Acq On : 26 May 2021 10:12  
Operator : JU/CG  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: May 26 11:03:30 2021  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF051421.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri May 14 19:05:57 2021  
Response via : Initial Calibration

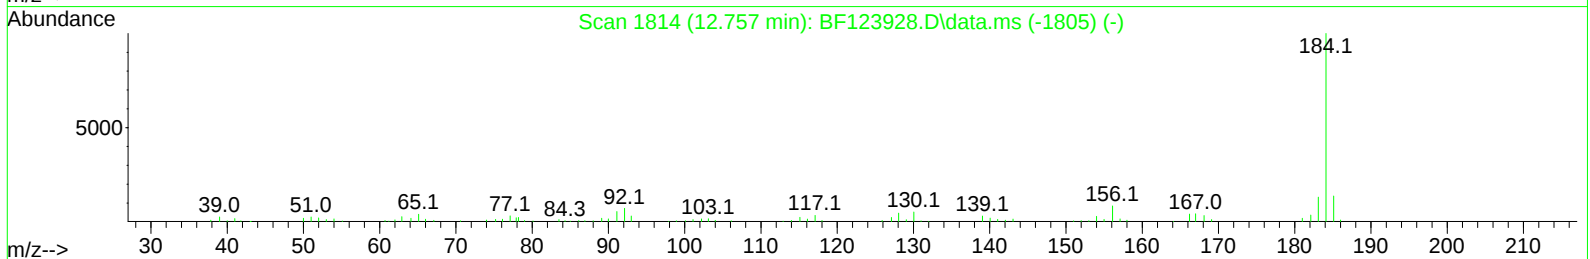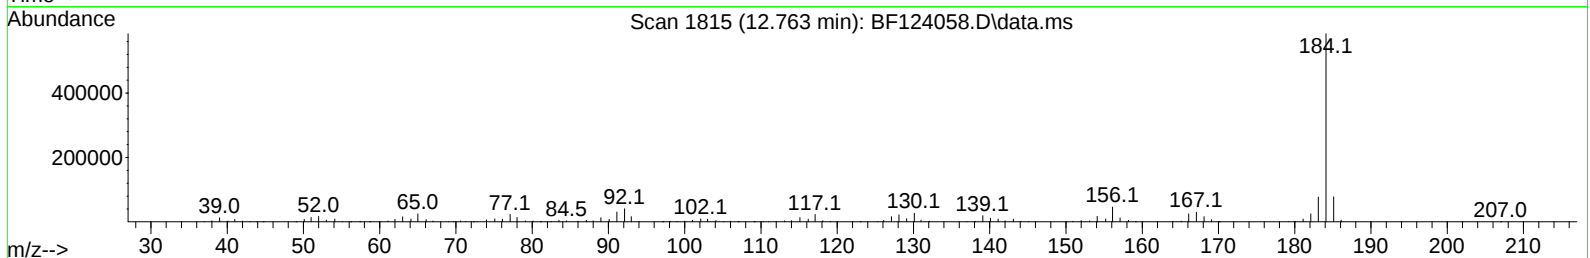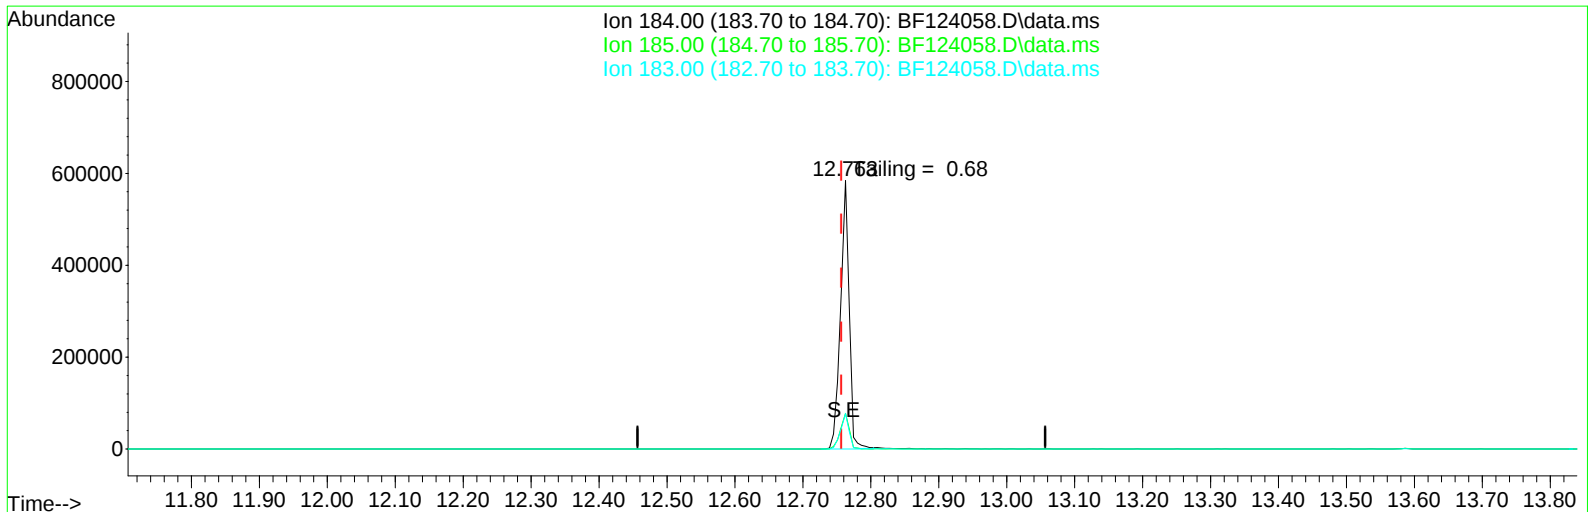

TIC: BF124058.D\data.ms

(77) Benzidine

12.763min (+ 0.006) 0.00 ng




response 523072

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.10  | 13.32  |
| 183.00 | 9.80   | 13.18# |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF052621\  
Data File : BF124058.D  
Acq On : 26 May 2021 10:12  
Operator : JU/CG  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: May 26 11:03:30 2021  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF051421.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri May 14 19:05:57 2021  
Response via : Initial Calibration

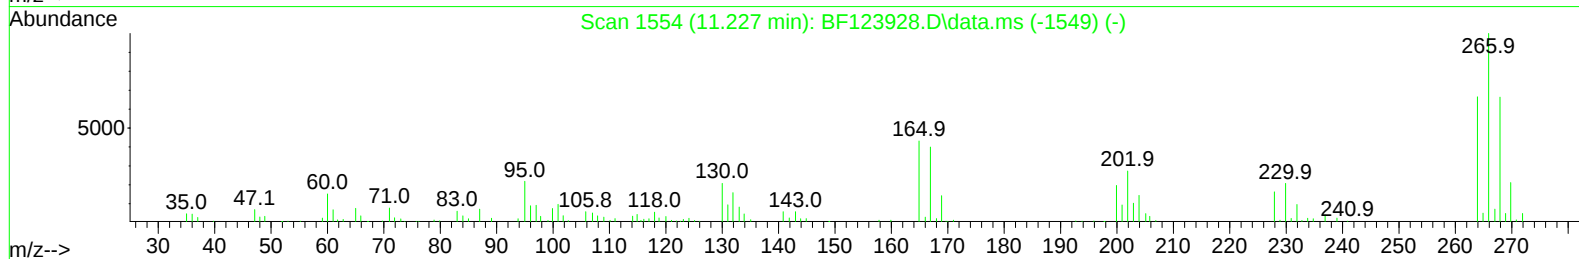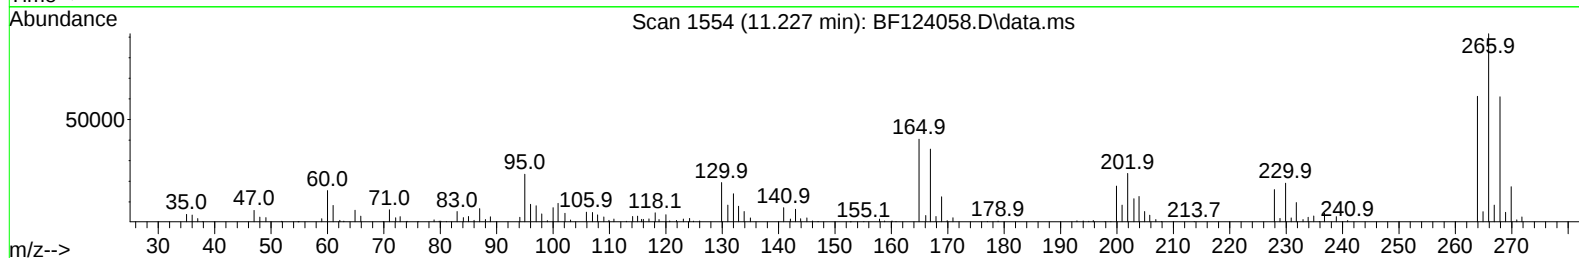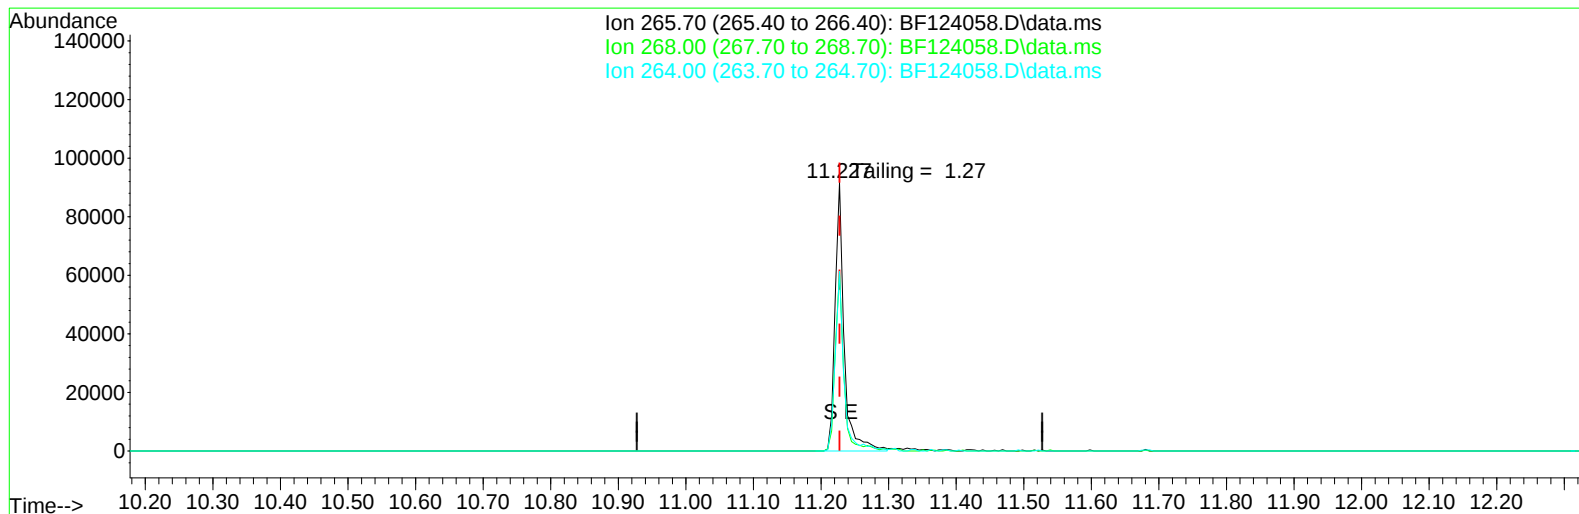

TIC: BF124058.D\data.ms

**(70) Pentachlorophenol (C)**

**11.227min (+ 0.000) 17378.70 ng**

**response 87370**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 64.50  | 66.57  |
| 264.00 | 65.70  | 66.88  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 5/26/2021     | BNA_F            | <u>BF124058.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 261019           | 13.58              |
| DDD           | 6972             | 13.28              |
| DDE           | 711              | 12.94              |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 7683          | 268702           | 2.86               |
|               |                  |                    |