
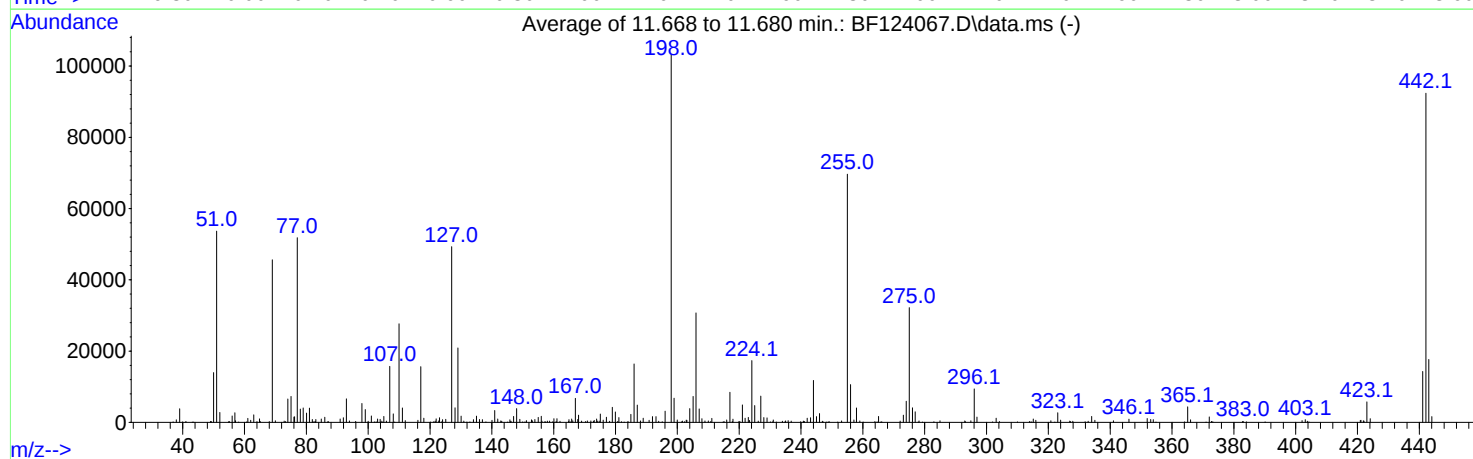


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052621\
 Data File : BF124067.D
 Acq On : 26 May 2021 16:26
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 27 13:12:25 2021

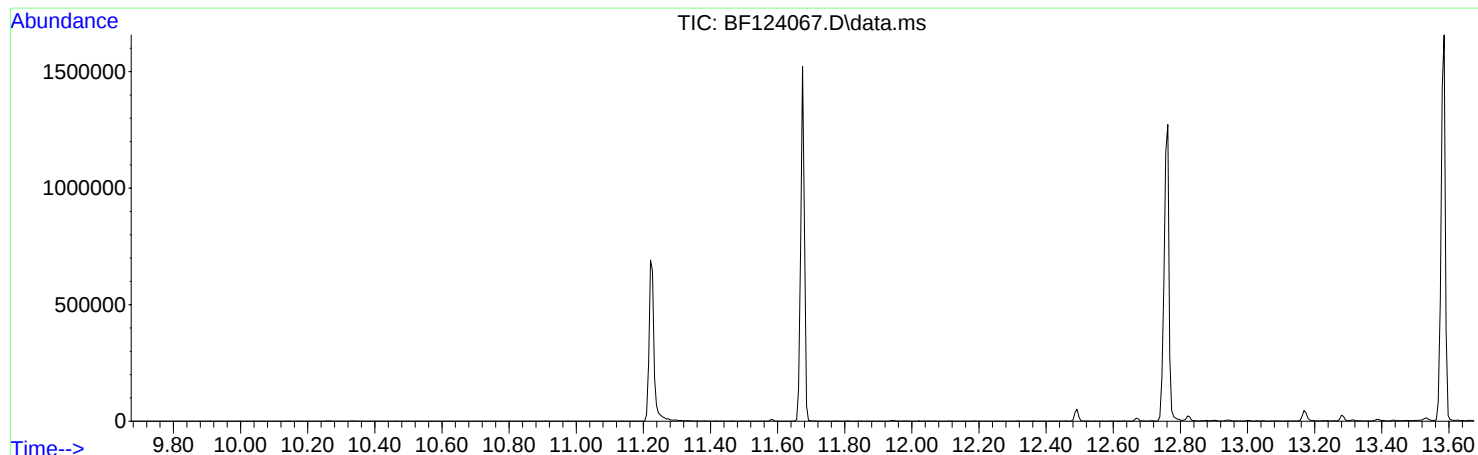




AutoFind: Scans 1629, 1630, 1631; Background Corrected with Scan 1624

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.0	53675	PASS
68	69	0.00	2	0.5	218	PASS
69	198	0.00	100	44.2	45635	PASS
70	69	0.00	2	1.0	453	PASS
127	198	10	80	47.8	49309	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	103251	PASS
199	198	5	9	6.6	6795	PASS
275	198	10	60	31.2	32181	PASS
365	198	1	100	4.2	4368	PASS
441	198	0.01	100	13.8	14279	PASS
442	442	50	100	100.0	92371	PASS
443	442	15	24	19.1	17657	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052621\
 Data File : BF124067.D
 Acq On : 26 May 2021 16:26
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 26 16:53:49 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 14 19:05:57 2021
 Response via : Initial Calibration

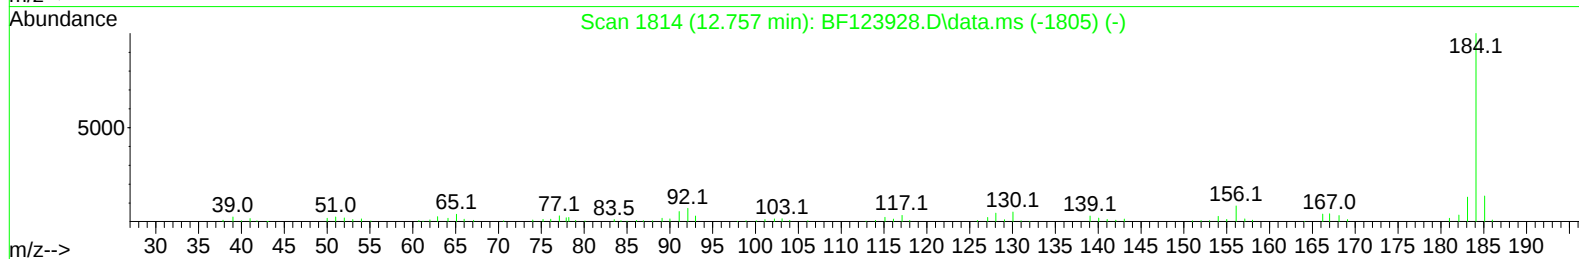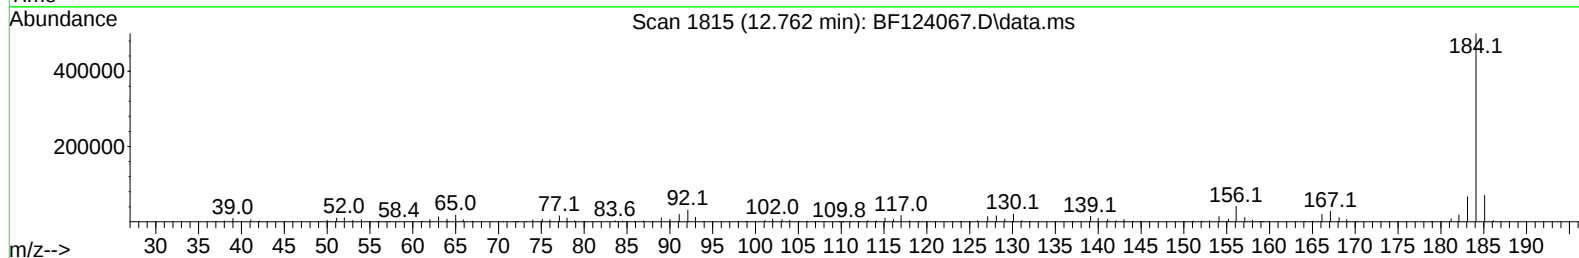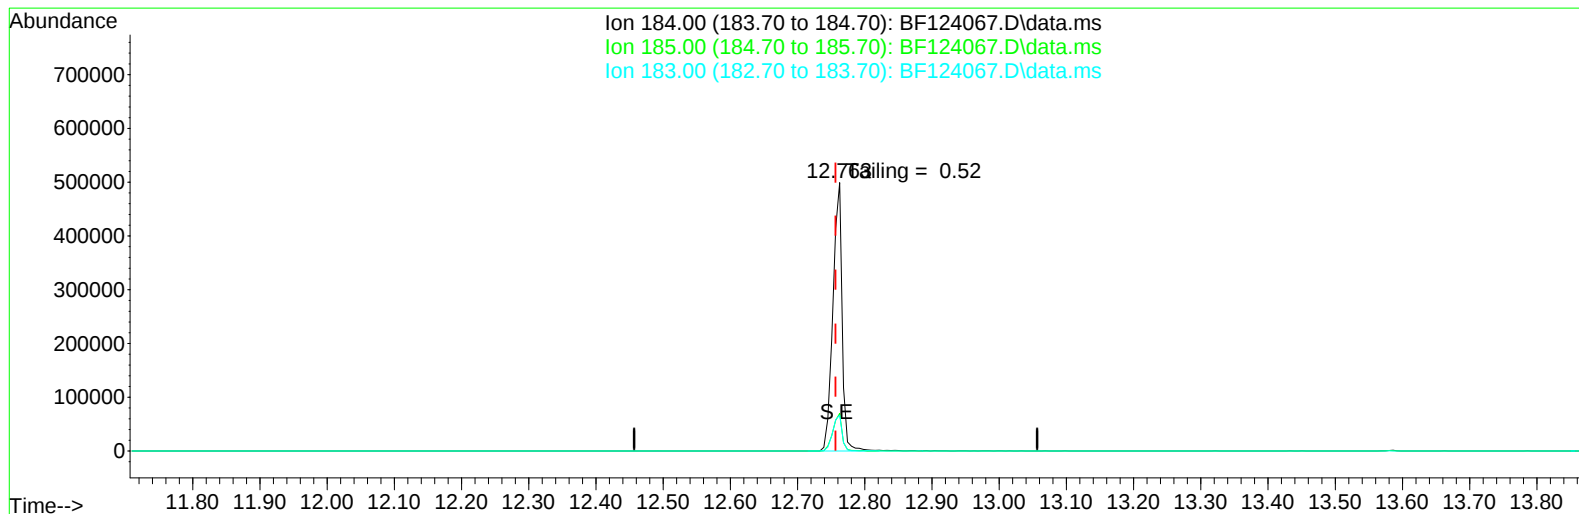

TIC: BF124067.D\data.ms

(77) Benzidine

12.762min (+ 0.006) 0.00 ng




response 478699

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.03
183.00	9.80	13.35#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052621\
Data File : BF124067.D
Acq On : 26 May 2021 16:26
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 26 16:53:49 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 19:05:57 2021
Response via : Initial Calibration

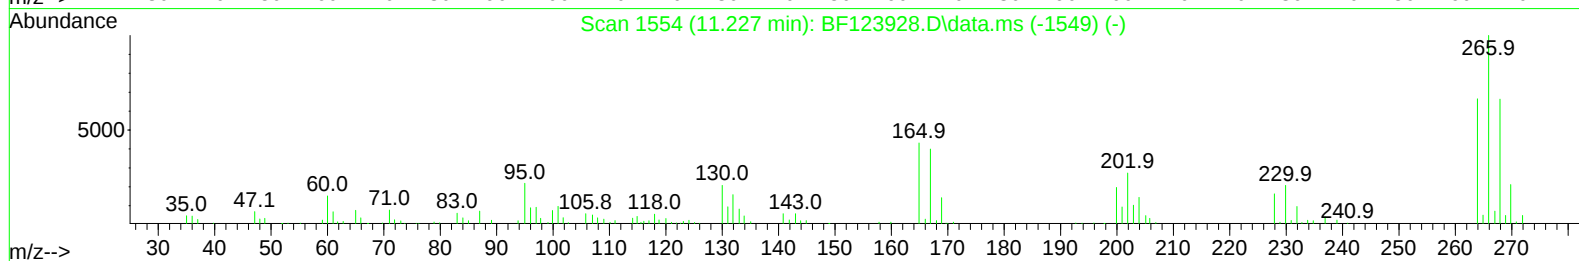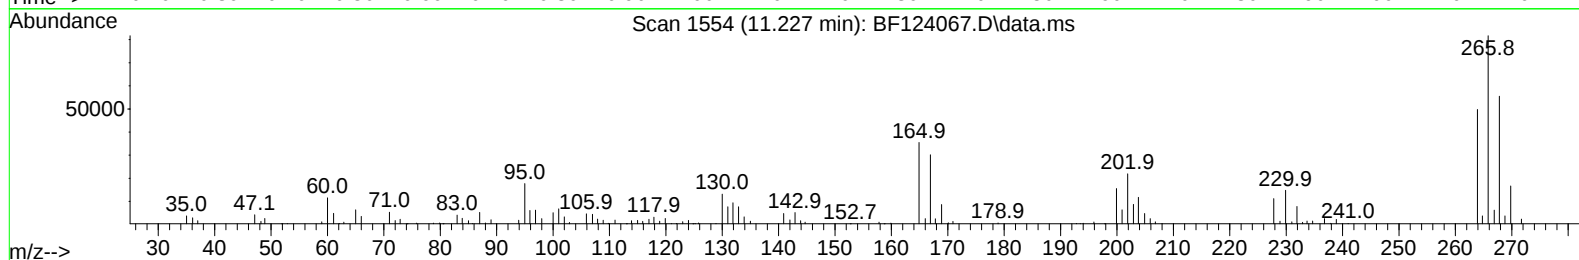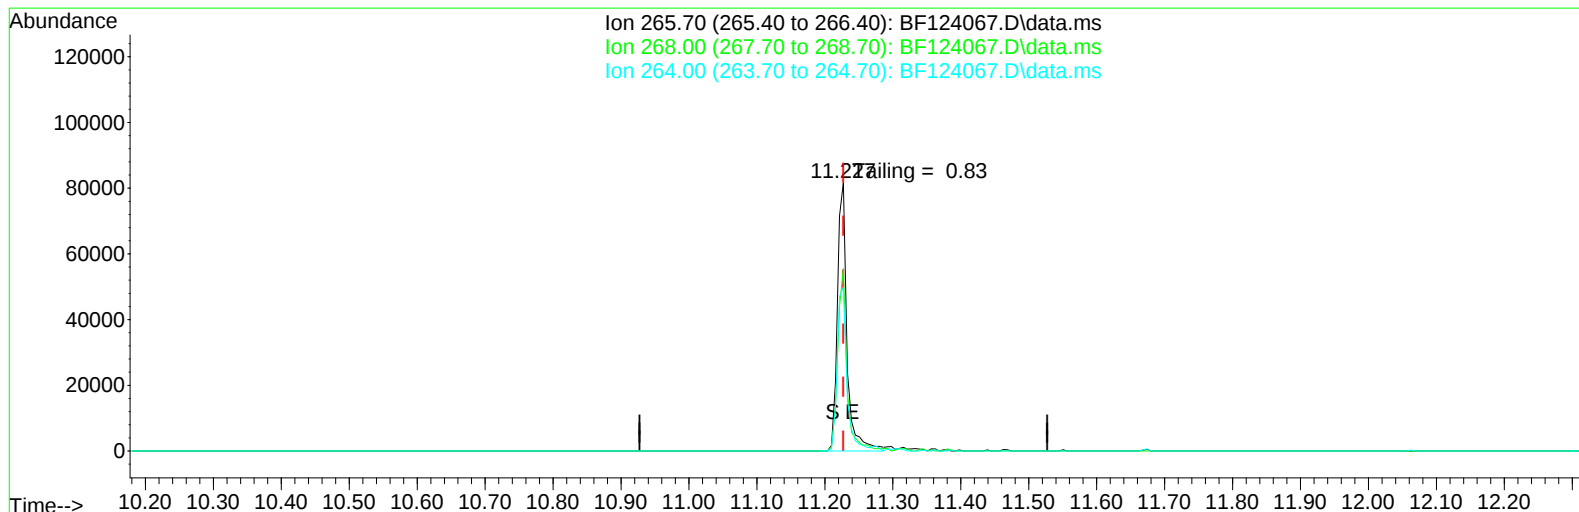

TIC: BF124067.D\data.ms

(70) Pentachlorophenol (C)

11.227min (-0.000) 21245.08 ng

response 82231

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	67.92
264.00	65.70	60.96
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/26/2021	BNA_F	<u>BF124067.D</u>
Compound Name	Response	Retention Time
DDT	267780	13.58
DDD	4669	13.28
DDE	899	12.94
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5568	273348	2.04