
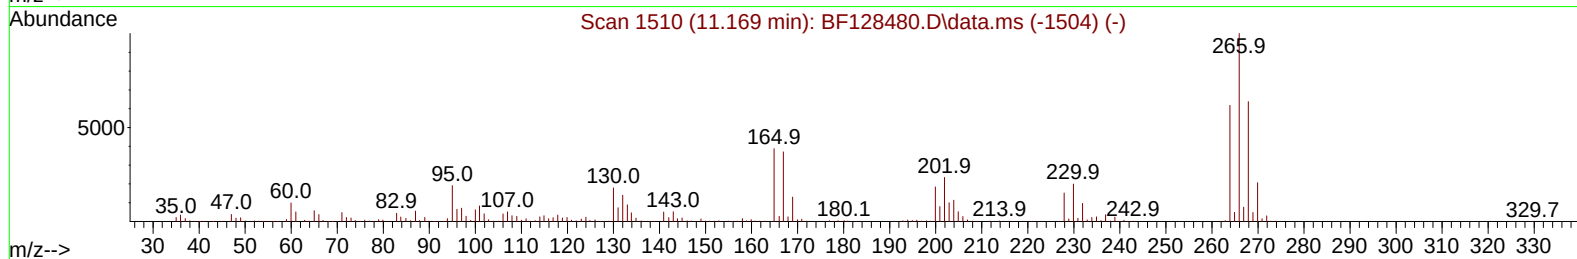
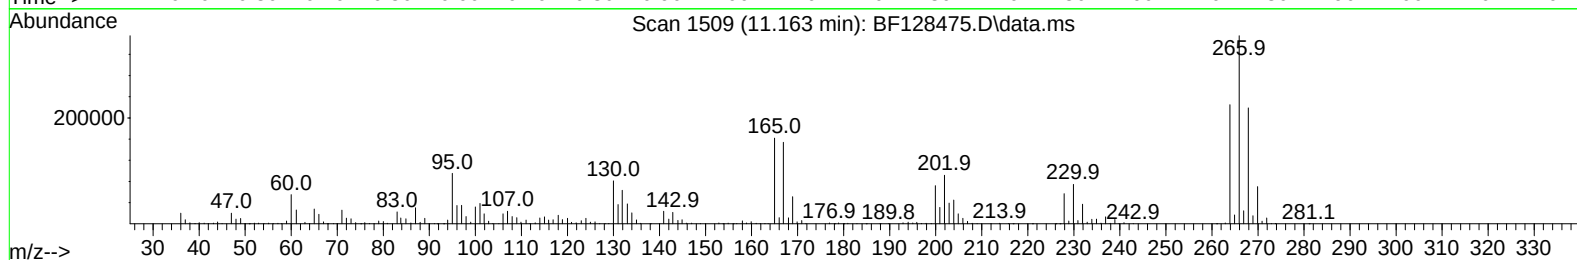


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052622\
Data File : BF128475.D
Acq On : 26 May 2022 16:00
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 27 07:36:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 27 01:51:59 2022
Response via : Initial Calibration

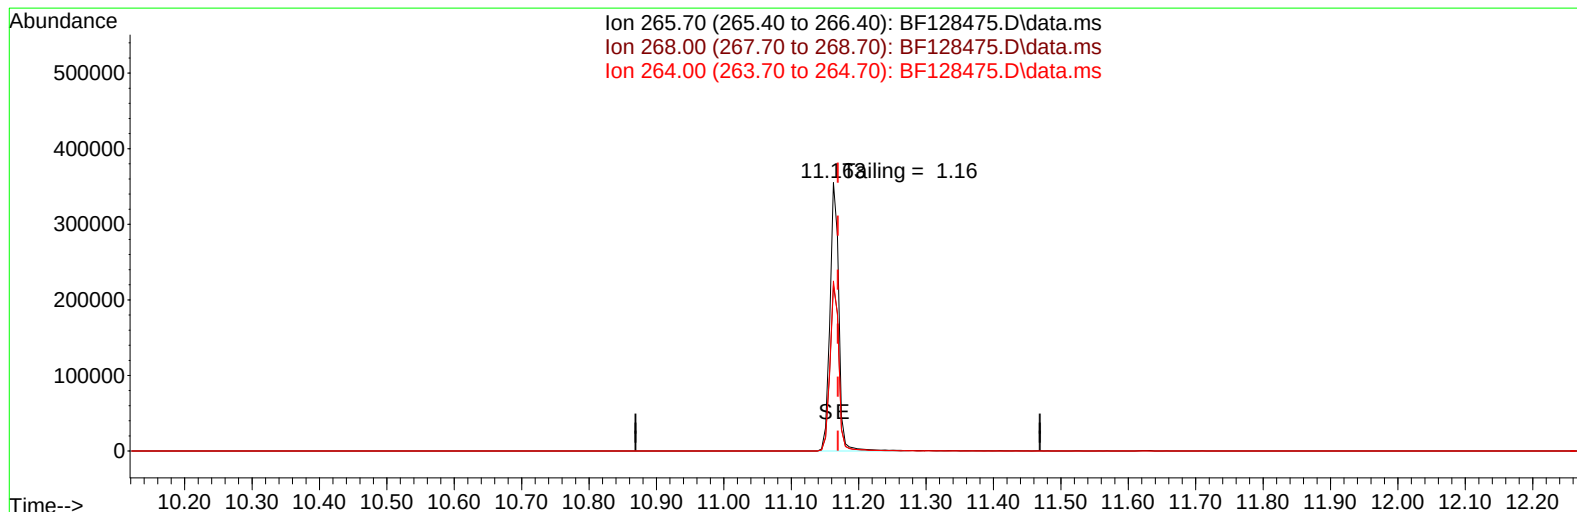

TIC: BF128475.D\data.ms

(70) Pentachlorophenol (C)




11.163min (-0.006) 386910.24 ng

response 325502

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	61.63
264.00	61.80	63.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052622\
 Data File : BF128475.D
 Acq On : 26 May 2022 16:00
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 27 07:36:20 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 27 01:51:59 2022
 Response via : Initial Calibration

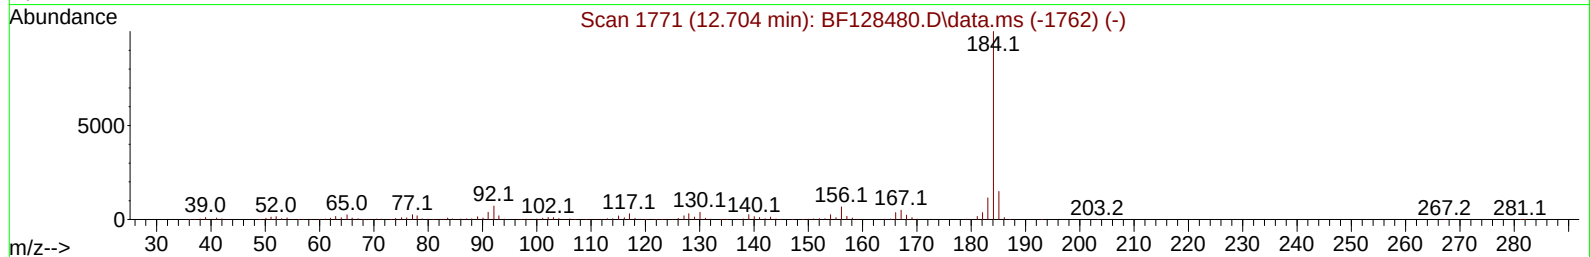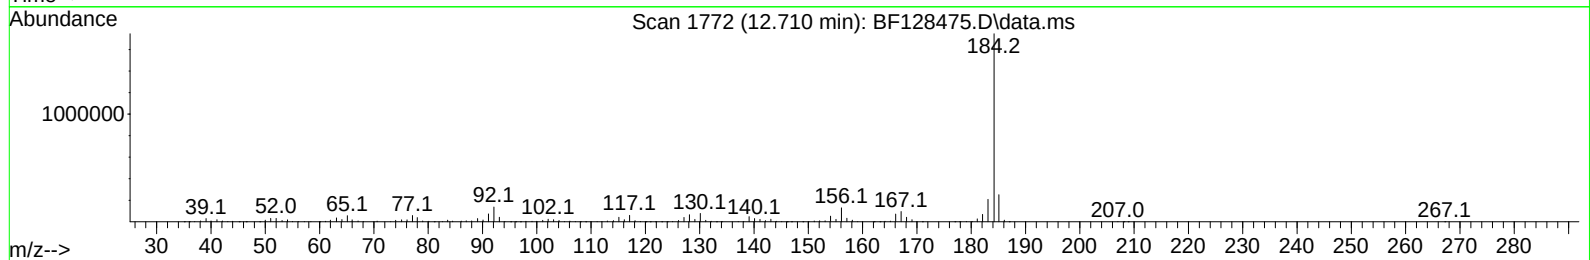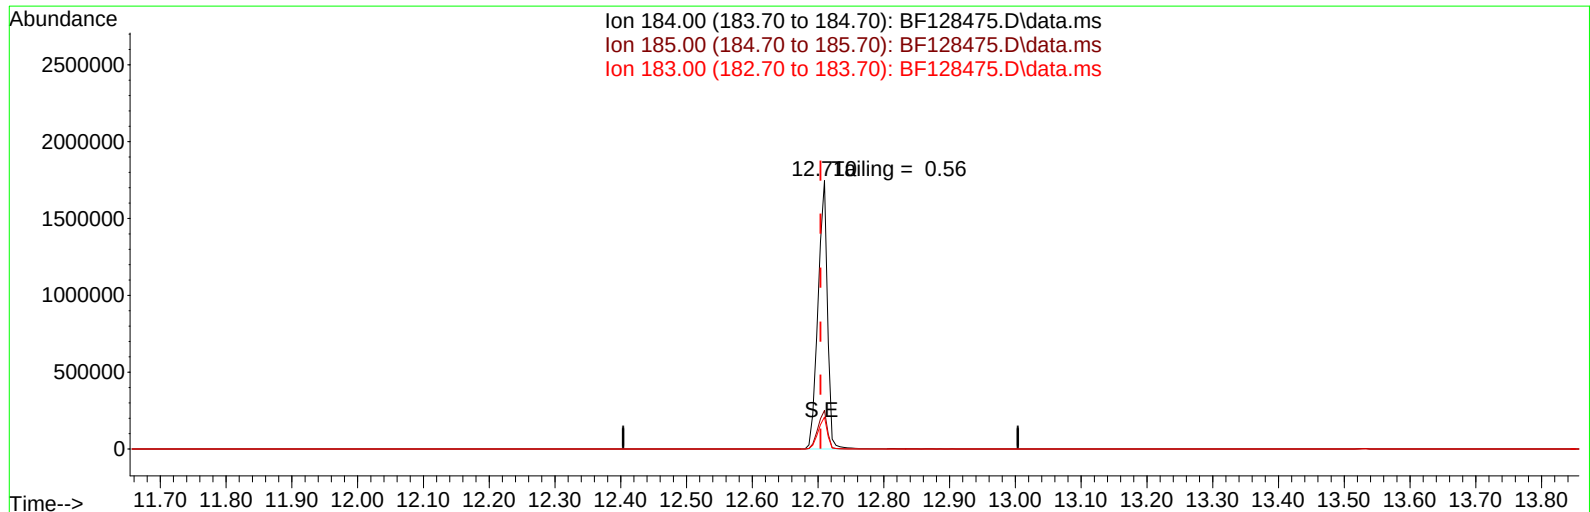

TIC: BF128475.D\data.ms

(77) Benzidine

12.710min (+ 0.006) 177280.10 ng

response 1741944

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.41
183.00	11.60	11.96
0.00	0.00	0.00