

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052622\
 Data File : BF128485.D
 Acq On : 26 May 2022 21:26
 Operator : CG\JU
 Sample : PB144997BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB144997BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128485.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.110	476	480	488	rVB	55706	82580	1.03%	0.159%
2	5.469	534	541	544	rBV	5383495	6555312	81.62%	12.640%
3	6.469	703	711	713	rBV	4815950	6626259	82.51%	12.777%
4	6.840	770	774	777	rVB	1648429	1402904	17.47%	2.705%
5	7.404	863	870	873	rBV	4048530	4501117	56.05%	8.679%
6	8.122	986	992	995	rBV	1833191	1908442	23.76%	3.680%
7	9.204	1168	1176	1179	rBV	6512707	8031115	100.00%	15.485%
8	9.875	1284	1290	1294	rBV	2520194	2330614	29.02%	4.494%
9	10.669	1417	1425	1428	rBV	4599589	4893173	60.93%	9.435%
10	11.363	1536	1543	1546	rBV	2689238	2323754	28.93%	4.481%
11	11.522	1566	1570	1573	rBV	99487	85446	1.06%	0.165%
12	12.963	1809	1815	1818	rVB	7081076	8024860	99.92%	15.473%
13	14.004	1988	1992	1995	rBV	2446268	2103216	26.19%	4.055%
14	14.104	2001	2009	2019	rBV	541702	726863	9.05%	1.402%
15	15.468	2235	2241	2246	rBV	1434314	1782570	22.20%	3.437%
16	16.968	2483	2496	2510	rVB3	99682	484337	6.03%	0.934%




Sum of corrected areas: 51862562

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052622\
Data File : BF128485.D
Acq On : 26 May 2022 21:26
Operator : CG\JU
Sample : PB144997BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144997BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

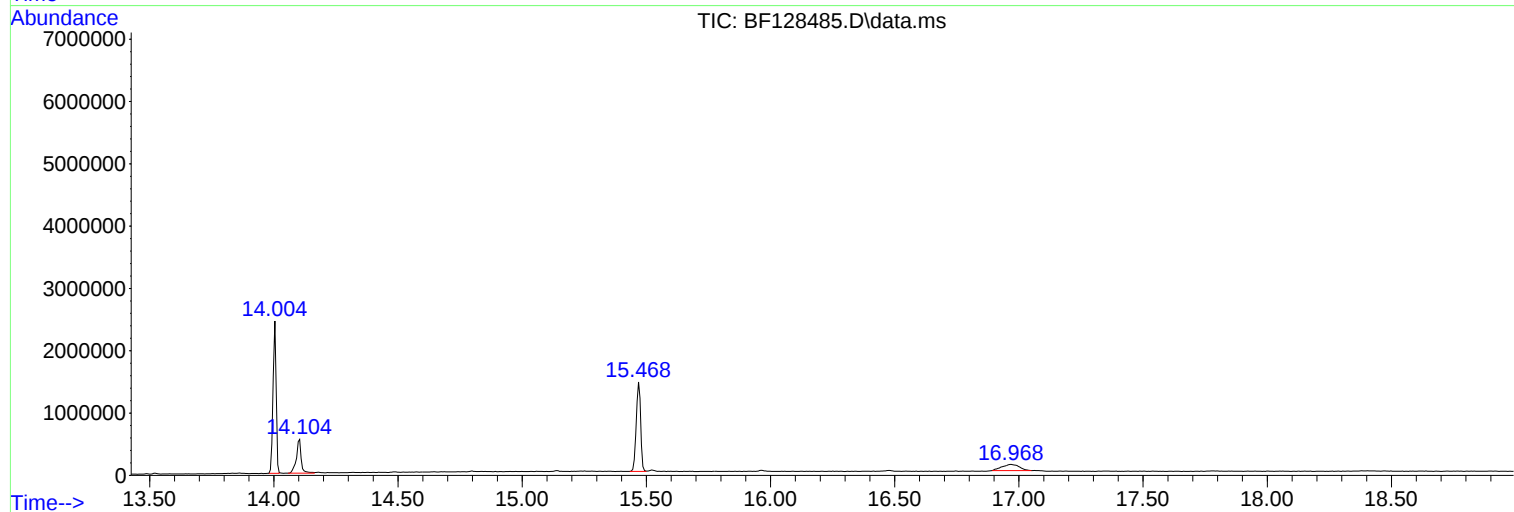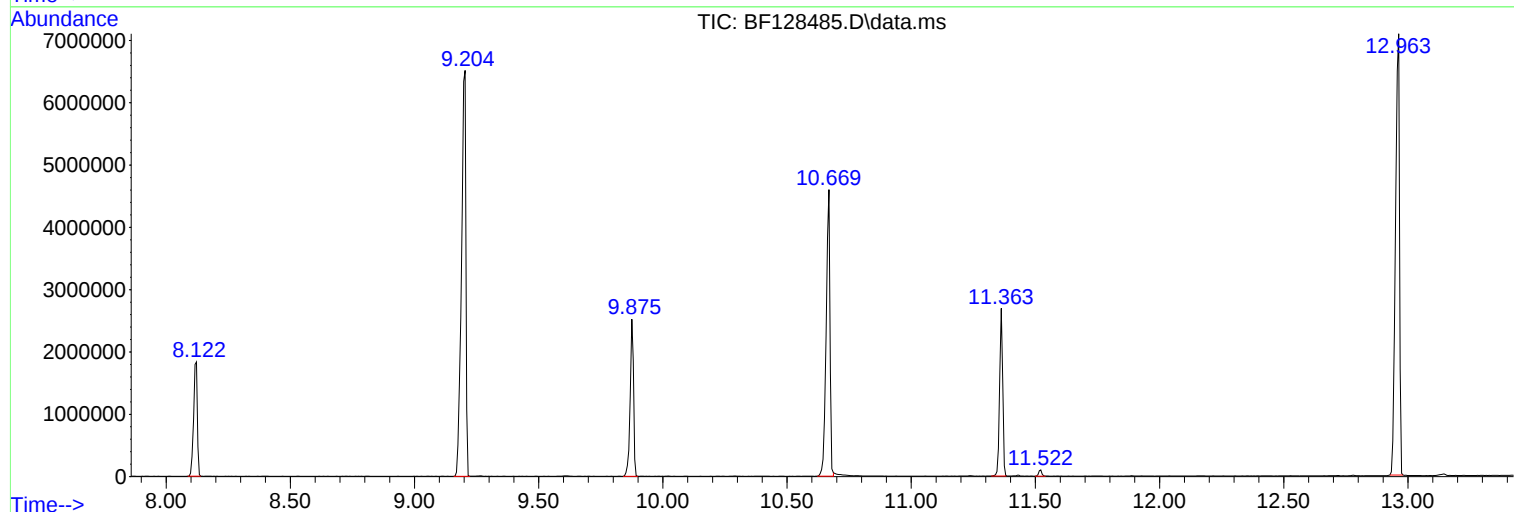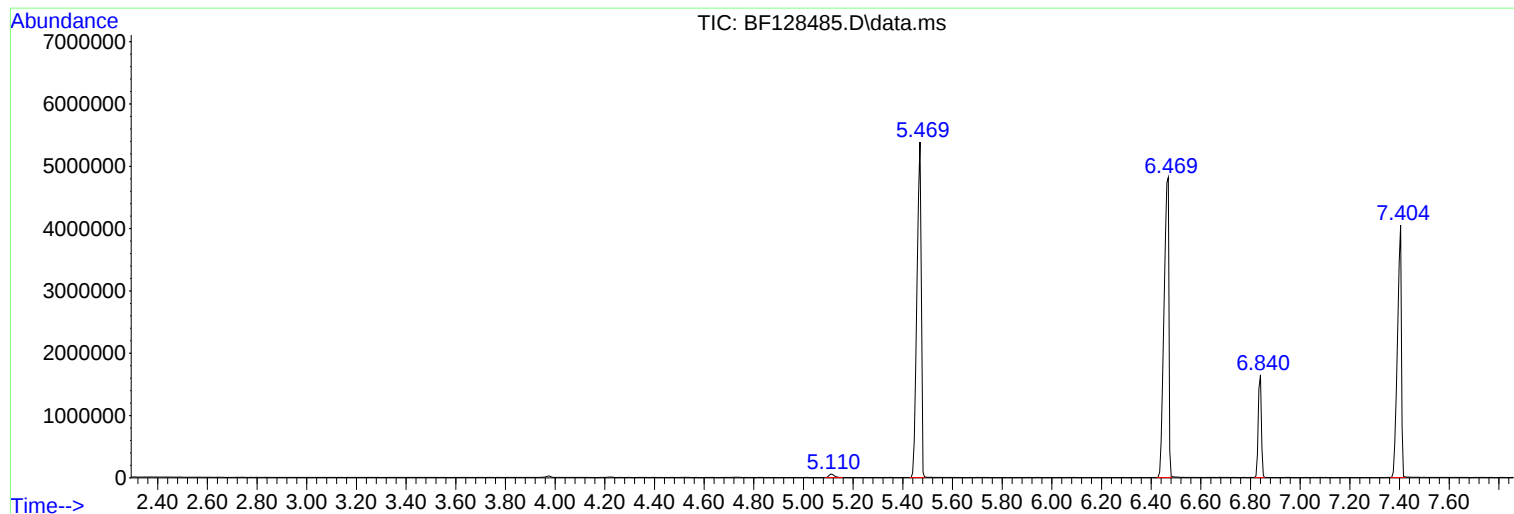

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052622\
Data File : BF128485.D
Acq On : 26 May 2022 21:26
Operator : CG\JU
Sample : PB144997BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144997BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052622\
Data File : BF128485.D
Acq On : 26 May 2022 21:26
Operator : CG\JU
Sample : PB144997BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144997BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------