

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052622\
 Data File : BF128486.D
 Acq On : 26 May 2022 21:56
 Operator : CG\JU
 Sample : PB145086BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB145086BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128486.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.110	475	480	488	rVB	54426	82511	1.02%	0.162%
2	5.469	534	541	544	rBV	5539607	6447328	79.48%	12.688%
3	6.469	703	711	713	rBV	4961299	6603352	81.41%	12.995%
4	6.840	770	774	777	rVB	1642437	1362678	16.80%	2.682%
5	7.404	863	870	873	rBV	3900753	4454525	54.92%	8.766%
6	8.122	987	992	995	rBV	1800408	1854632	22.86%	3.650%
7	9.204	1169	1176	1179	rBV	6503920	7934010	97.81%	15.613%
8	9.875	1284	1290	1294	rBV	2407693	2183511	26.92%	4.297%
9	10.669	1417	1425	1428	rBV	4796885	4913766	60.58%	9.670%
10	11.363	1537	1543	1546	rBV	2669867	2296137	28.31%	4.519%
11	12.963	1809	1815	1818	rBV	7322351	8111470	100.00%	15.962%
12	14.004	1988	1992	1995	rBV	2378817	2089001	25.75%	4.111%
13	14.098	2002	2008	2018	rBV	570992	715349	8.82%	1.408%
14	15.468	2235	2241	2246	rBV	1438318	1767870	21.79%	3.479%




Sum of corrected areas: 50816140

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052622\
Data File : BF128486.D
Acq On : 26 May 2022 21:56
Operator : CG\JU
Sample : PB145086BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145086BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

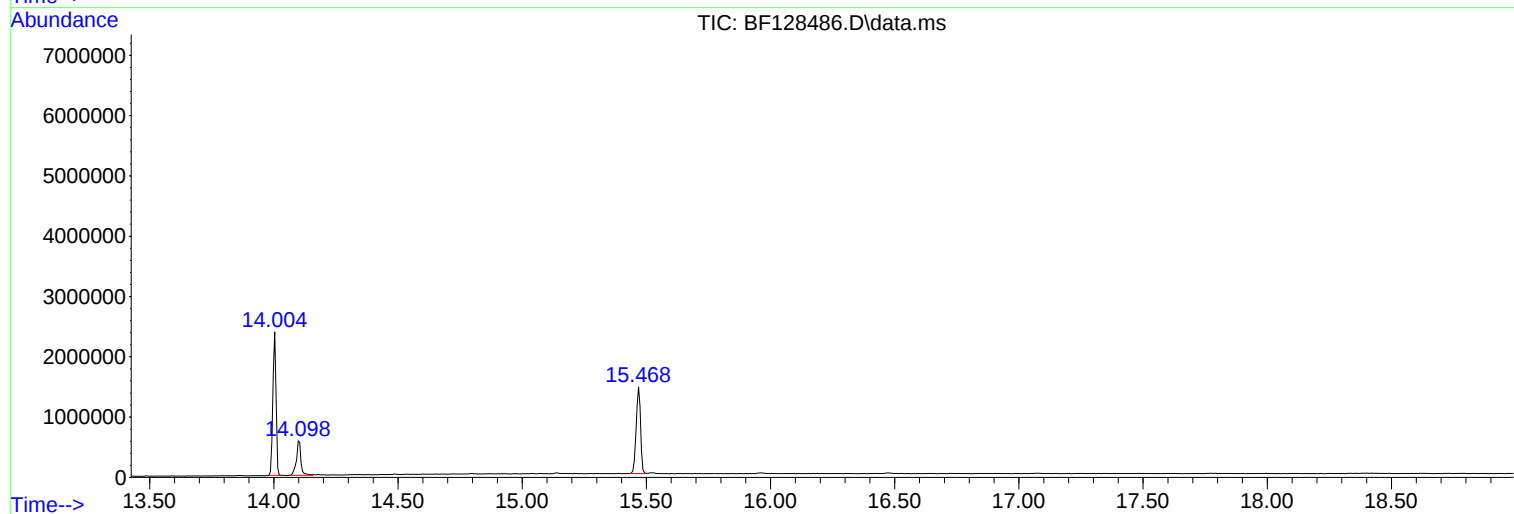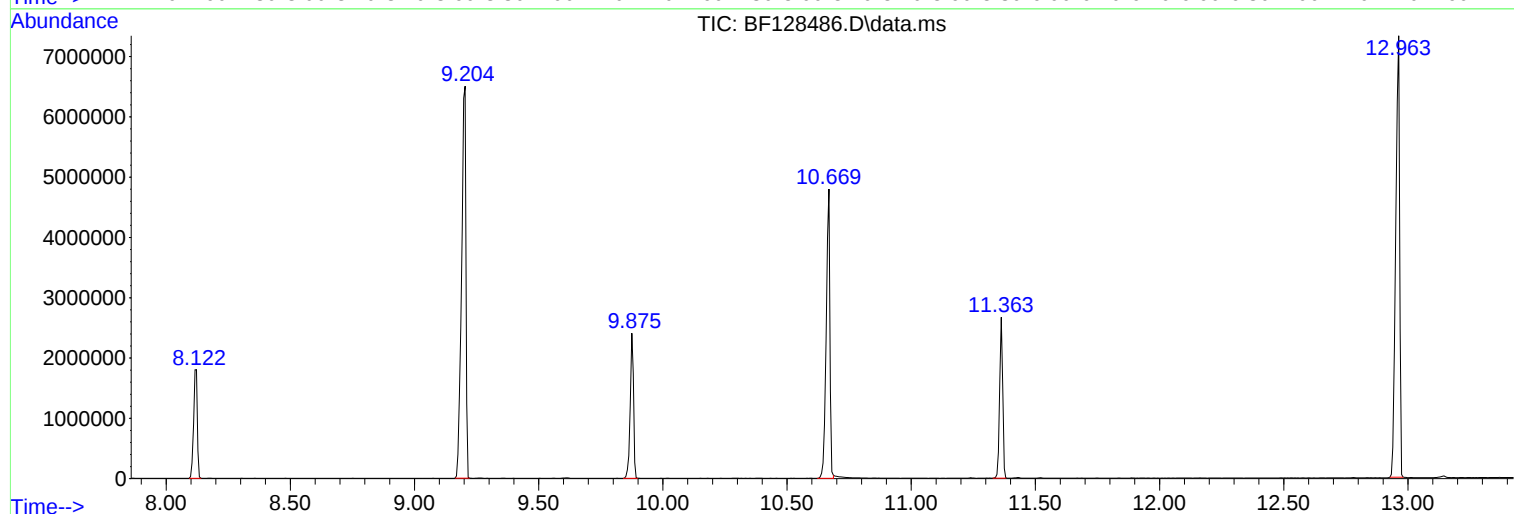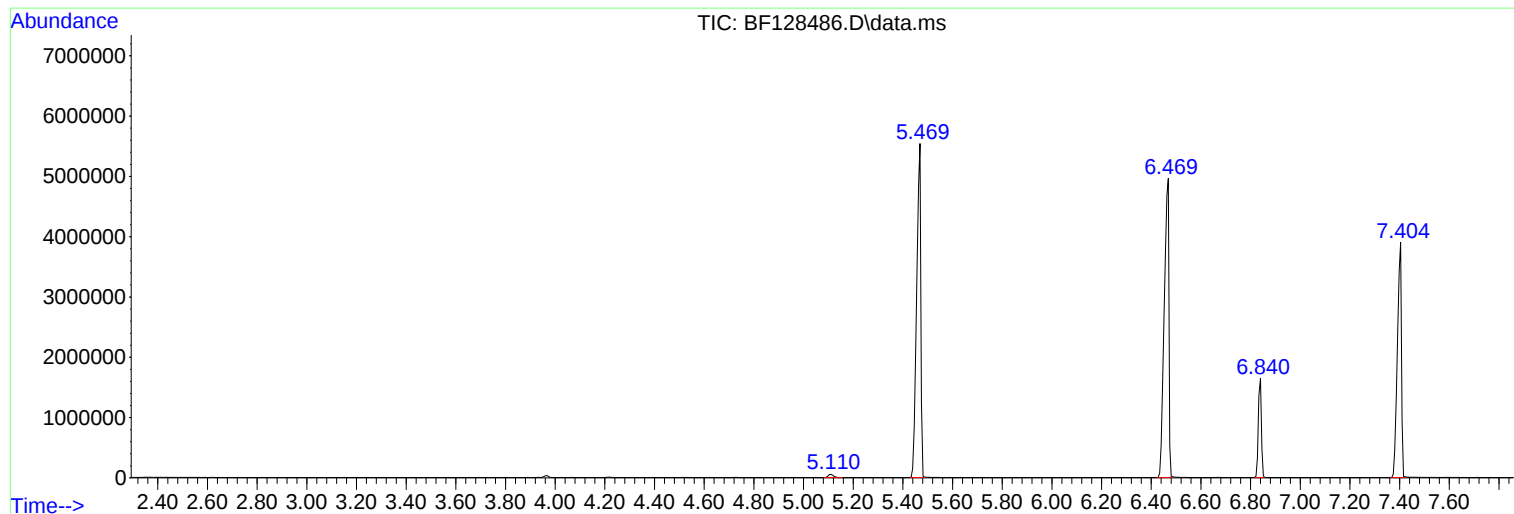

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052622\
Data File : BF128486.D
Acq On : 26 May 2022 21:56
Operator : CG\JU
Sample : PB145086BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145086BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.098	6.85 ng	715349	Chrysene-d12	14.004

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	93
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19NO3S	1000483-83-4	87
3			Formaldehyde, (triphenylphosphor...]	304	C19H17N2P	015990-54-2	50
4			4-Nitro-4'-methyldiphenylsulfone	277	C13H11NO4S	004094-37-5	43
5			Carbazol-1-one, 1,2,3,4-tetrahyd...	277	C18H15NO2	299962-12-2	32

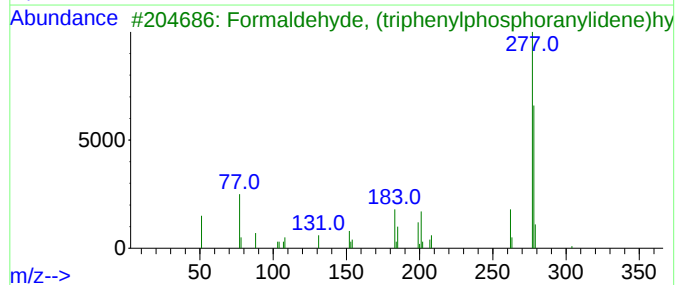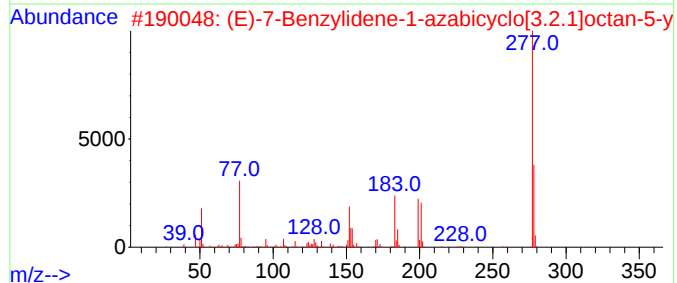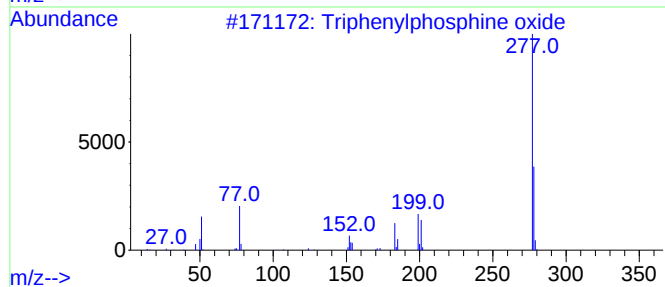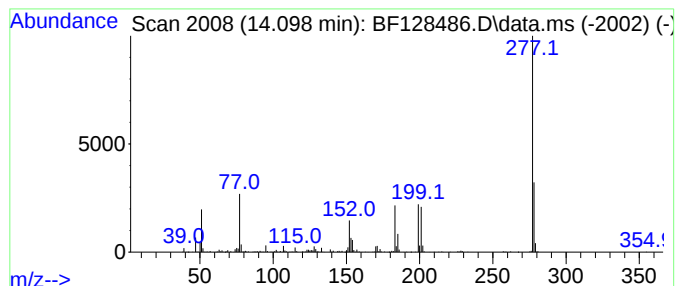

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052622\
Data File : BF128486.D
Acq On : 26 May 2022 21:56
Operator : CG\JU
Sample : PB145086BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145086BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.098	6.8	ng	715349	5	14.004	2089000	20.0