

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052622\
 Data File : BF128488.D
 Acq On : 26 May 2022 22:55
 Operator : CG\JU
 Sample : PB145123BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB145123BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128488.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.469	534	541	544	rBV	5514503	6489964	82.04%	12.903%
2	6.469	703	711	713	rBV	4763605	6631805	83.84%	13.185%
3	6.840	770	774	777	rBV	1626887	1369080	17.31%	2.722%
4	7.404	863	870	873	rBV	4030264	4485115	56.70%	8.917%
5	8.116	986	991	995	rBV	1810135	1863382	23.56%	3.705%
6	9.198	1169	1175	1179	rBV	6609584	7910312	100.00%	15.727%
7	9.875	1281	1290	1293	rBV	2423188	2167212	27.40%	4.309%
8	10.669	1417	1425	1428	rBV	4566259	4843799	61.23%	9.630%
9	11.363	1537	1543	1546	rBV	2616322	2252544	28.48%	4.478%
10	12.963	1809	1815	1818	rVB	7208769	7849416	99.23%	15.606%
11	14.004	1987	1992	1995	rBV	2223733	2017259	25.50%	4.011%
12	14.098	2002	2008	2019	rBV	557389	718452	9.08%	1.428%
13	15.468	2235	2241	2246	rBV	1368449	1700114	21.49%	3.380%




Sum of corrected areas: 50298454

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052622\
Data File : BF128488.D
Acq On : 26 May 2022 22:55
Operator : CG\JU
Sample : PB145123BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145123BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

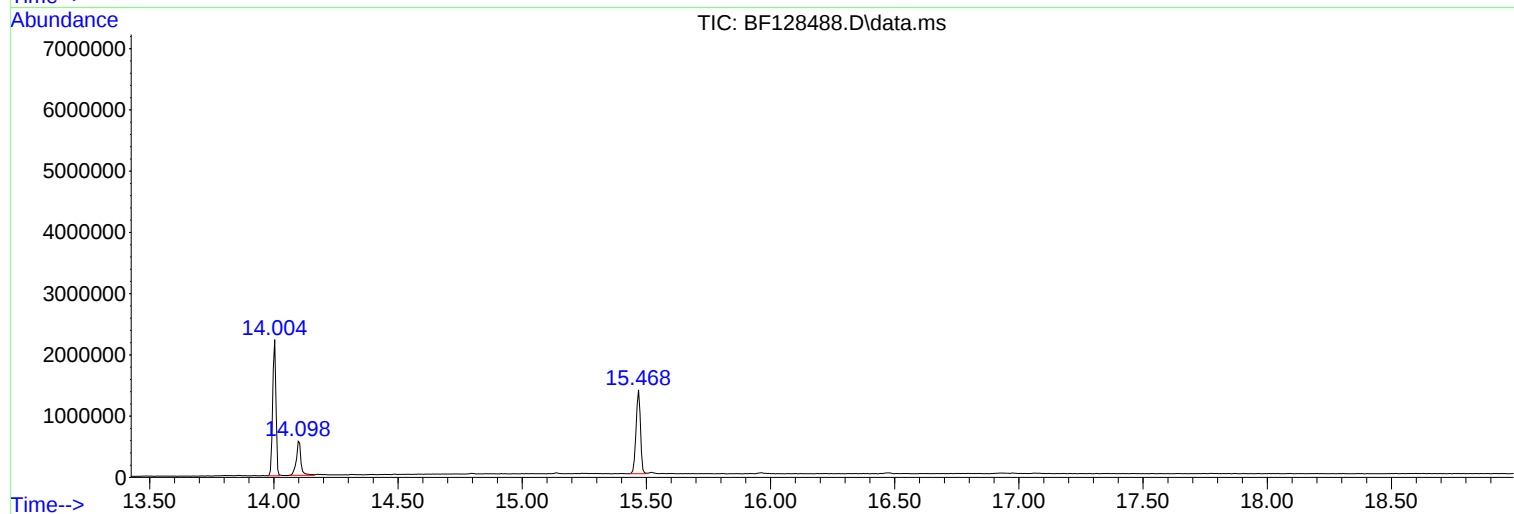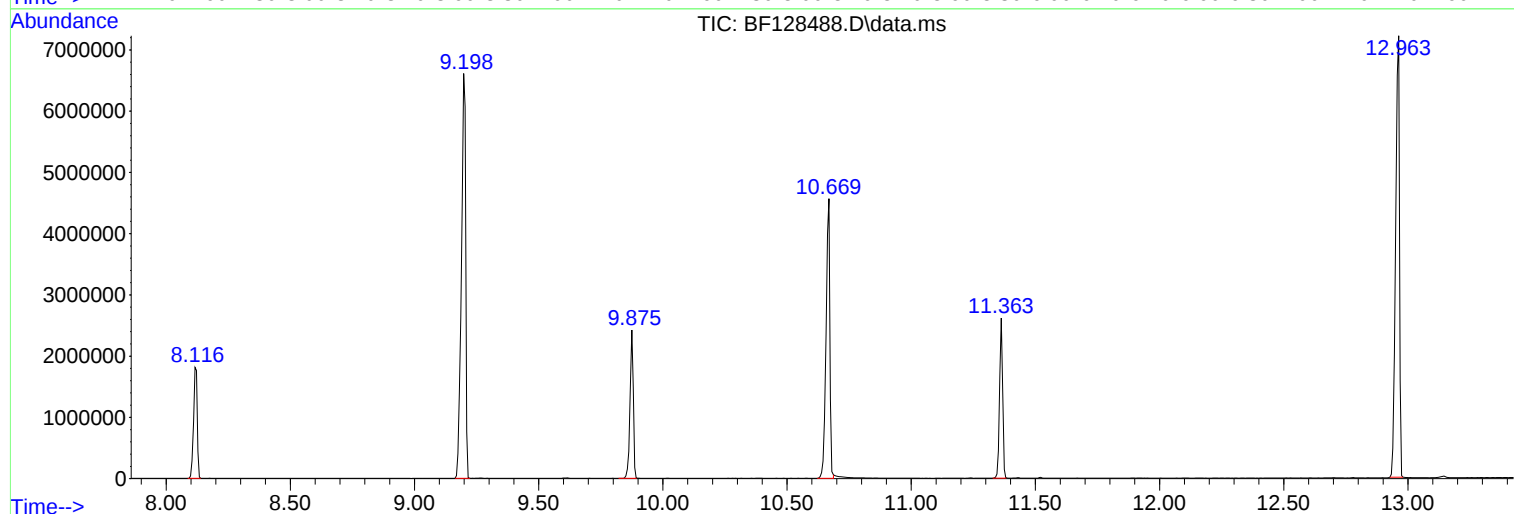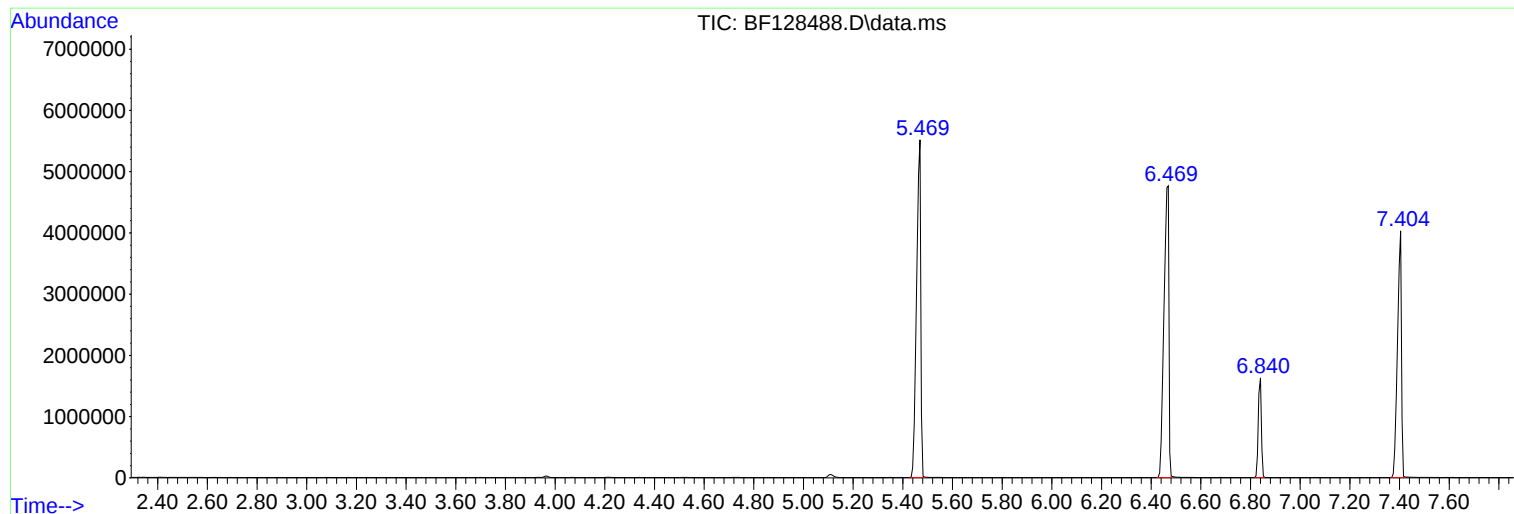

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052622\
Data File : BF128488.D
Acq On : 26 May 2022 22:55
Operator : CG\JU
Sample : PB145123BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145123BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052622\
Data File : BF128488.D
Acq On : 26 May 2022 22:55
Operator : CG\JU
Sample : PB145123BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145123BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------