

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052622\
 Data File : BF128490.D
 Acq On : 26 May 2022 23:54
 Operator : CG\JU
 Sample : PB145002BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB145002BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128490.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.122	478	482	489	rVB	61470	91935	1.01%	0.157%
2	5.469	534	541	544	rBV	5808157	7544439	82.51%	12.872%
3	6.469	703	711	714	rBV	5574460	7555902	82.63%	12.892%
4	6.840	770	774	777	rBV	1985221	1639910	17.93%	2.798%
5	7.404	863	870	873	rBV	4331043	5248924	57.40%	8.956%
6	8.122	986	992	995	rBV	2208403	2248841	24.59%	3.837%
7	9.204	1168	1176	1179	rBV	7367339	9143972	100.00%	15.602%
8	9.875	1284	1290	1294	rBV	2722043	2604805	28.49%	4.444%
9	10.669	1415	1425	1428	rBV	5073200	5518759	60.35%	9.416%
10	11.363	1536	1543	1546	rBV	3076066	2692561	29.45%	4.594%
11	11.522	1566	1570	1573	rBV	121369	112137	1.23%	0.191%
12	12.963	1809	1815	1818	rBV	7943397	9102228	99.54%	15.530%
13	14.004	1988	1992	1995	rBV	2671722	2386072	26.09%	4.071%
14	14.098	2001	2008	2019	rBV	538979	717273	7.84%	1.224%
15	15.468	2235	2241	2247	rBV2	1612650	2001397	21.89%	3.415%




Sum of corrected areas: 58609155

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052622\
Data File : BF128490.D
Acq On : 26 May 2022 23:54
Operator : CG\JU
Sample : PB145002BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145002BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

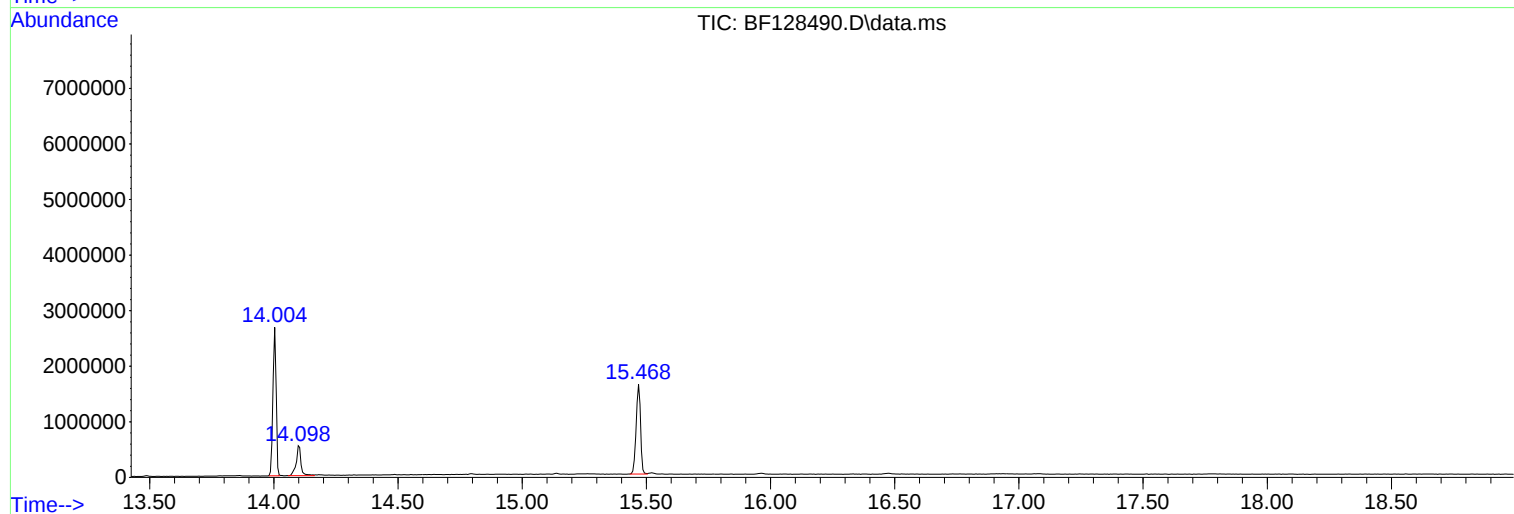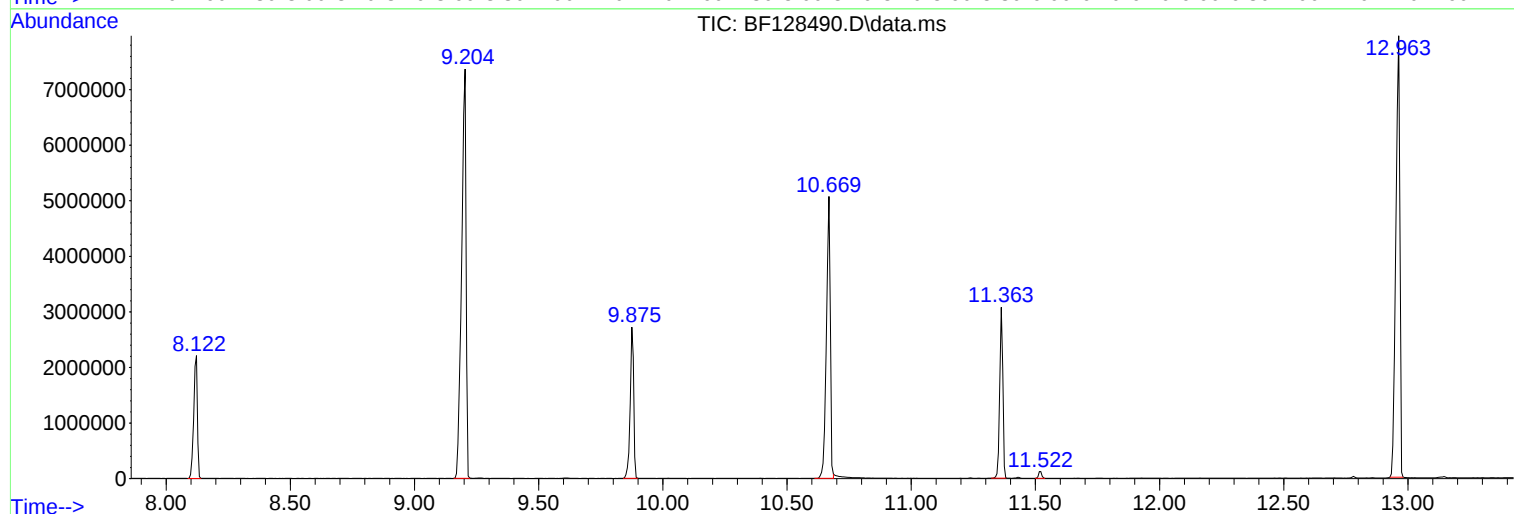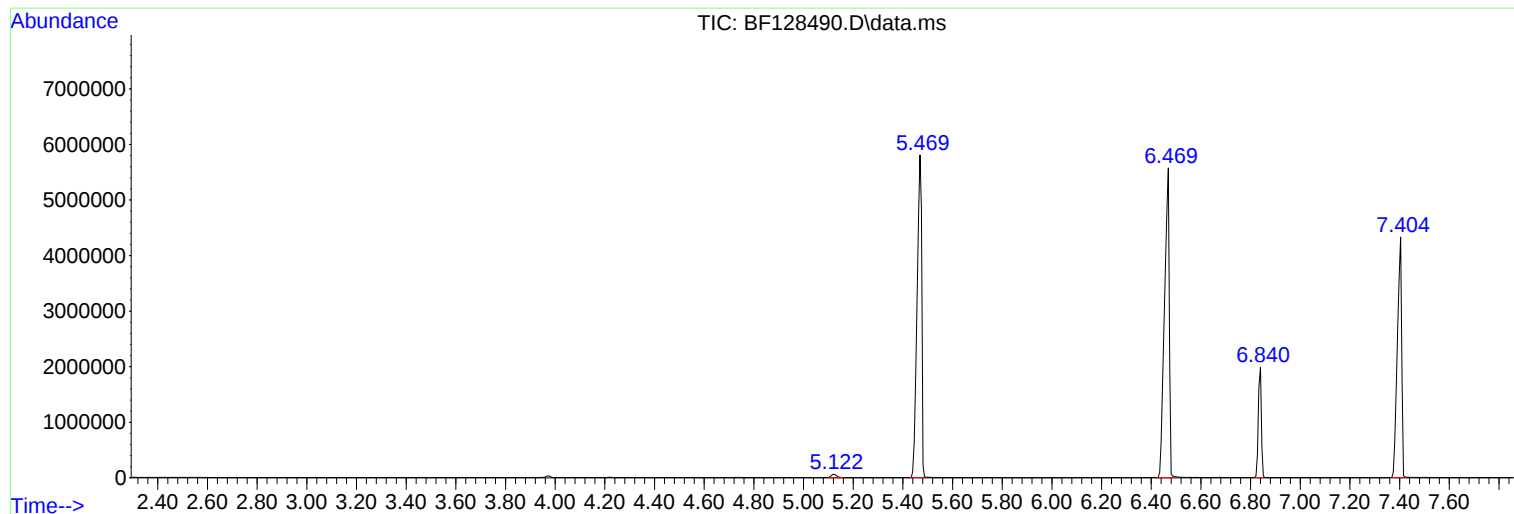

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052622\
Data File : BF128490.D
Acq On : 26 May 2022 23:54
Operator : CG\JU
Sample : PB145002BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145002BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.098	6.01 ng	717273	Chrysene-d12	14.004

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	93
2			(E)-7-Benzylidene-1-azabicyclo[3.2.1]octan-5-ylidene	293	C15H19NO3S	1000483-83-4	70
3			4-Nitro-4'-methyldiphenylsulfone	277	C13H11NO4S	004094-37-5	46
4			Formaldehyde, (triphenylphosphor...) (triphenylphosphorane)	304	C19H17N2P	015990-54-2	45
5			Carbazol-1-one, 1,2,3,4-tetrahyd...	277	C18H15NO2	299962-12-2	38

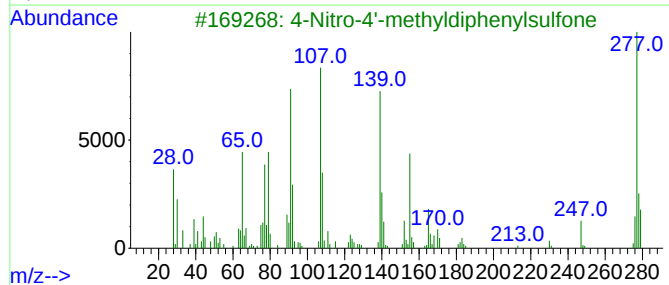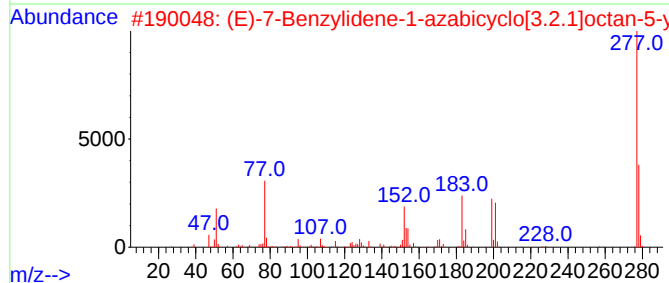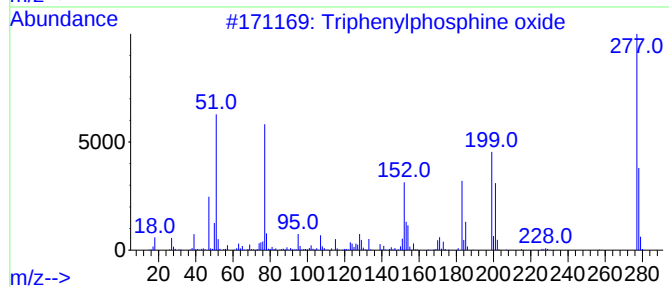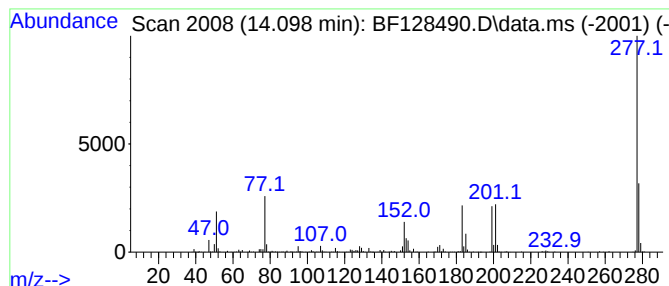

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052622\
Data File : BF128490.D
Acq On : 26 May 2022 23:54
Operator : CG\JU
Sample : PB145002BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145002BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.098	6.0	ng	717273	5	14.004	2386070	20.0