

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052622\
 Data File : BF128492.D
 Acq On : 27 May 2022 00:53
 Operator : CG\JU
 Sample : PB145064BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB145064BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128492.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.463	534	540	543	rBV	5334431	6902724	82.13%	13.234%
2	6.469	703	711	713	rBV	5199464	6948329	82.68%	13.321%
3	6.840	770	774	777	rVB	1618050	1357960	16.16%	2.603%
4	7.404	863	870	873	rBV	4219592	4770848	56.77%	9.146%
5	8.122	986	992	995	rBV	1859828	1855063	22.07%	3.556%
6	9.204	1169	1176	1179	rBV	6916200	8254618	98.22%	15.825%
7	9.875	1284	1290	1294	rBV	2477263	2173728	25.86%	4.167%
8	10.669	1417	1425	1428	rBV	4954847	5049527	60.08%	9.681%
9	11.363	1537	1543	1546	rBV	2707708	2240134	26.66%	4.295%
10	12.963	1809	1815	1818	rBV	7379305	8404133	100.00%	16.112%
11	14.004	1988	1992	1995	rBV	2167403	1950448	23.21%	3.739%
12	14.098	2002	2008	2016	rBV	540888	669315	7.96%	1.283%
13	15.468	2235	2241	2248	rBV	1276966	1583806	18.85%	3.036%




Sum of corrected areas: 52160633

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052622\
Data File : BF128492.D
Acq On : 27 May 2022 00:53
Operator : CG\JU
Sample : PB145064BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145064BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

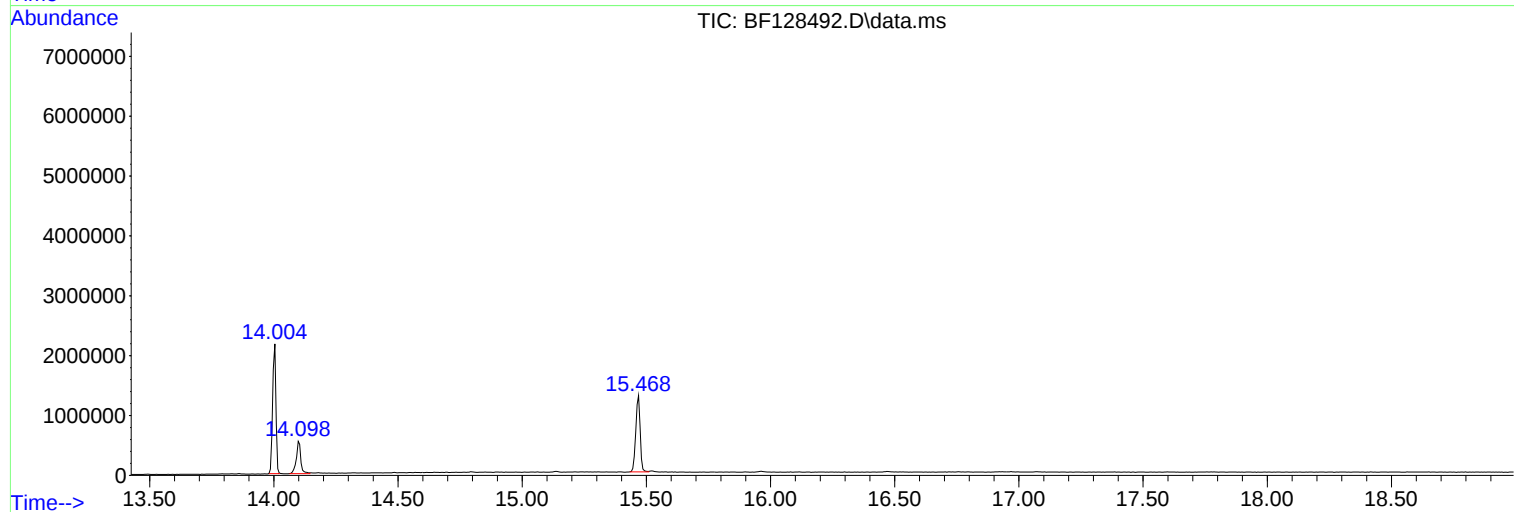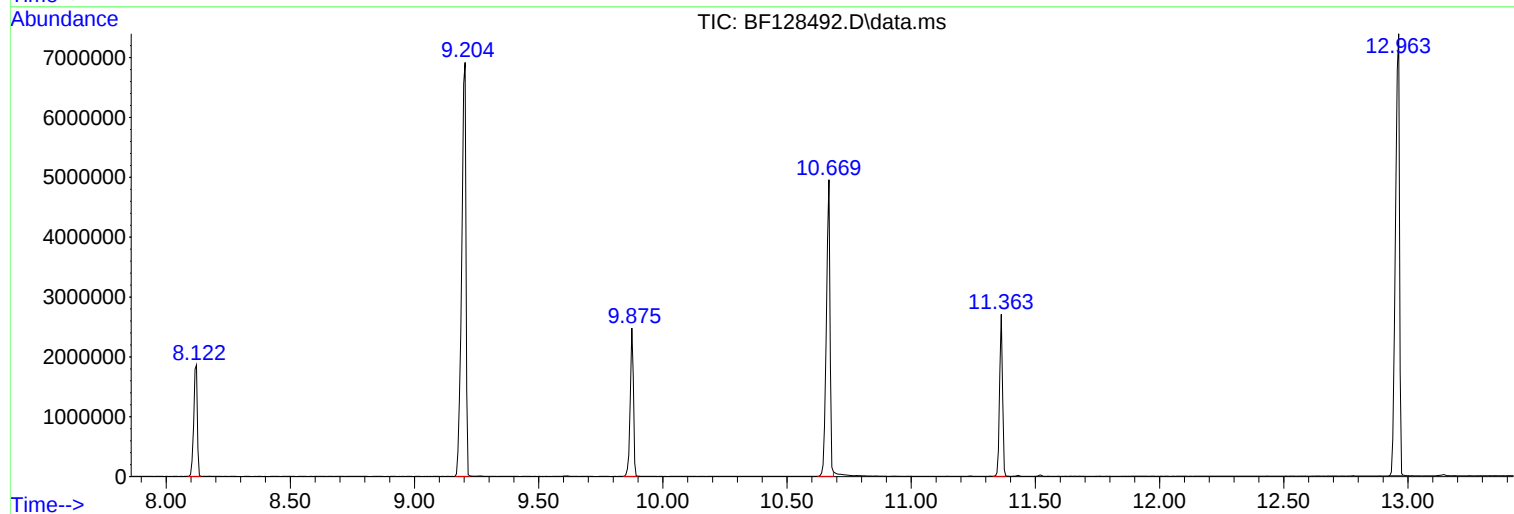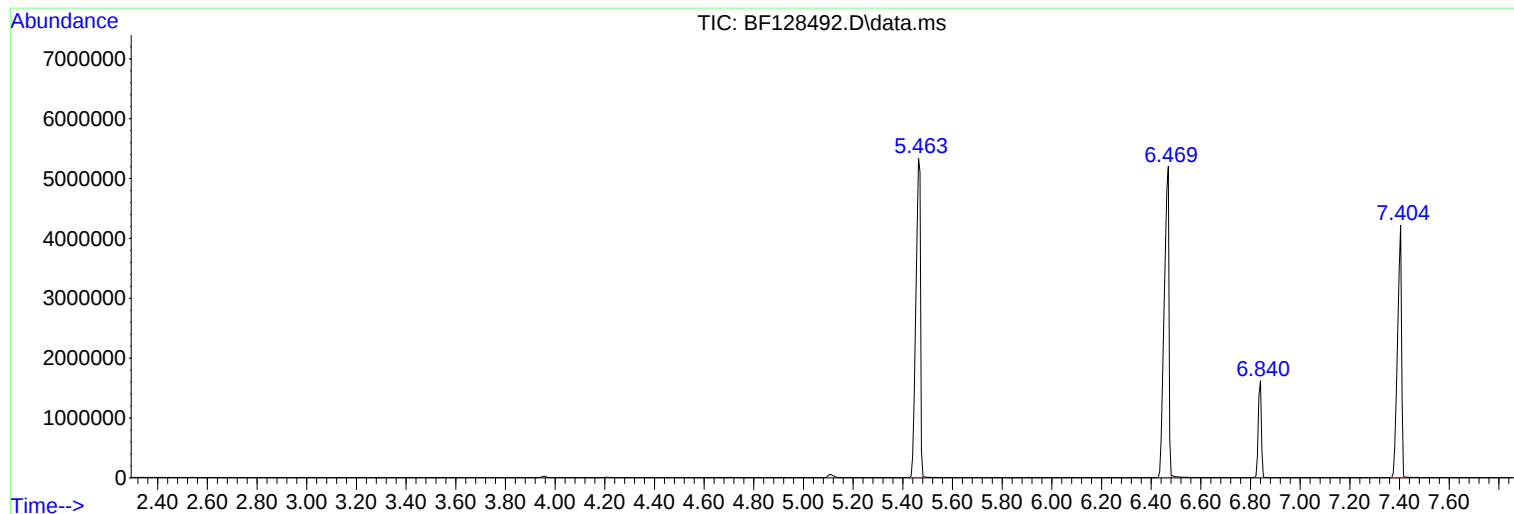

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052622\
Data File : BF128492.D
Acq On : 27 May 2022 00:53
Operator : CG\JU
Sample : PB145064BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145064BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052622\
Data File : BF128492.D
Acq On : 27 May 2022 00:53
Operator : CG\JU
Sample : PB145064BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145064BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------