

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052622\
 Data File : BF128494.D
 Acq On : 27 May 2022 01:52
 Operator : CG\JU
 Sample : PB145118BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB145118BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128494.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.128	479	483	489	rBV	67134	99508	1.02%	0.168%
2	5.475	534	542	545	rBV	6085313	8073459	82.70%	13.667%
3	6.469	703	711	714	rBV	5610949	8206410	84.06%	13.893%
4	6.840	770	774	777	rVB	1547271	1322607	13.55%	2.239%
5	7.404	863	870	873	rBV	4517288	5677994	58.16%	9.612%
6	8.116	986	991	995	rBV	1829153	1828858	18.73%	3.096%
7	9.204	1168	1176	1179	rBV	7780191	9727487	99.64%	16.468%
8	9.875	1284	1290	1294	rBV	2309777	2120602	21.72%	3.590%
9	10.669	1417	1425	1428	rBV	5323094	5930245	60.74%	10.039%
10	11.363	1536	1543	1546	rBV	2547788	2197238	22.51%	3.720%
11	12.963	1806	1815	1818	rBV	8126784	9762587	100.00%	16.527%
12	14.004	1987	1992	1995	rBV	2043267	1916955	19.64%	3.245%
13	14.098	2001	2008	2017	rBV	556841	683449	7.00%	1.157%
14	15.468	2235	2241	2247	rBV	1271723	1523234	15.60%	2.579%




Sum of corrected areas: 59070633

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052622\
Data File : BF128494.D
Acq On : 27 May 2022 01:52
Operator : CG\JU
Sample : PB145118BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145118BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

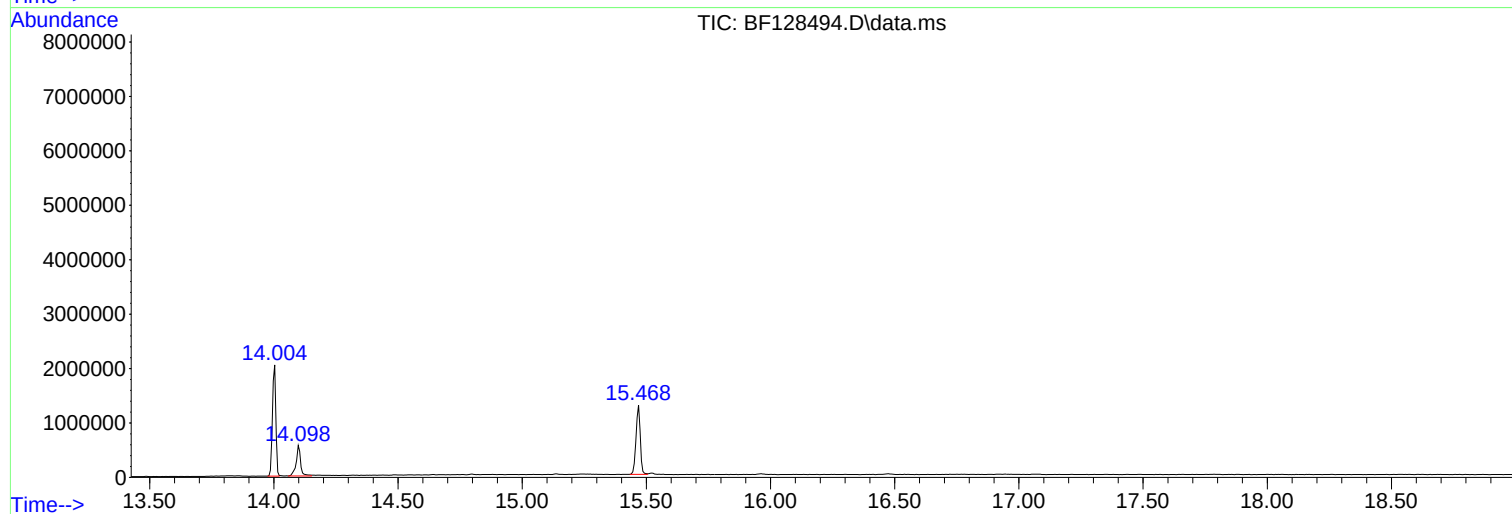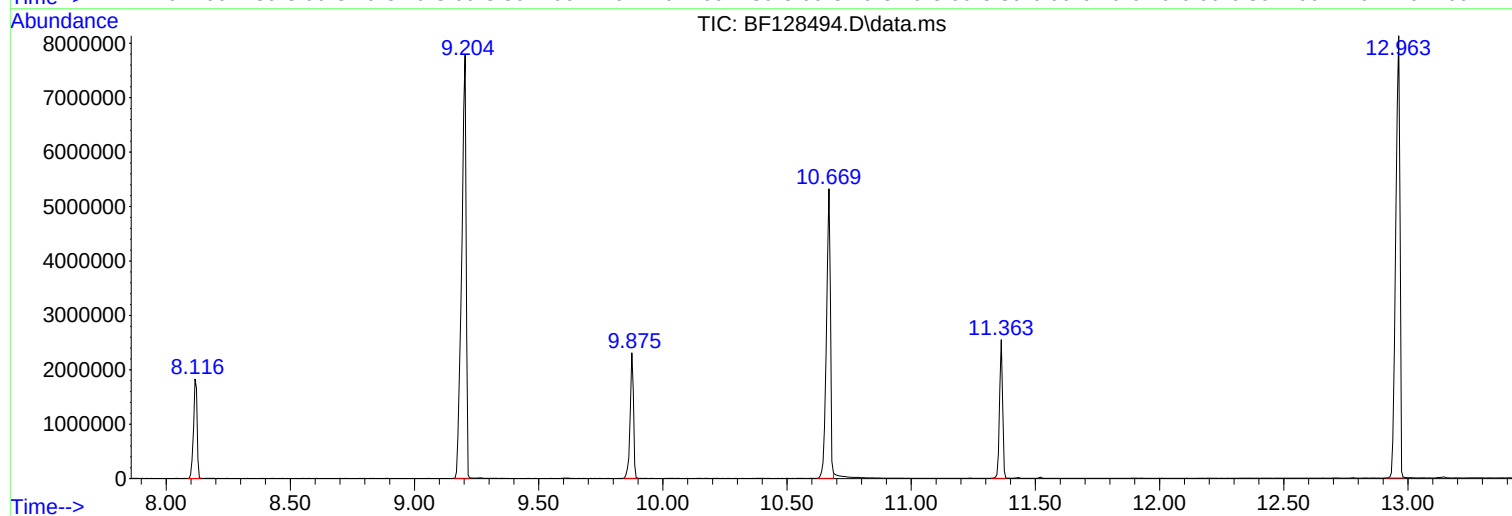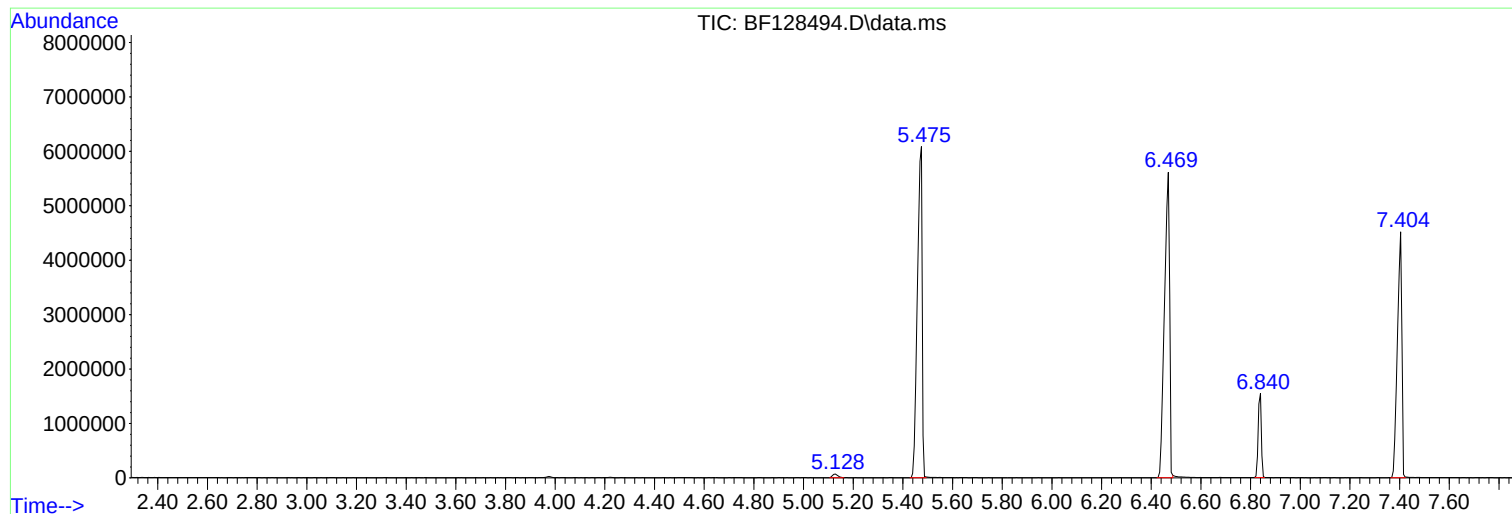

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052622\
Data File : BF128494.D
Acq On : 27 May 2022 01:52
Operator : CG\JU
Sample : PB145118BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145118BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.098	7.13 ng	683449	Chrysene-d12	14.004

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	93
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19NO3S	1000483-83-4	87
3			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	64
4			Carbazol-1-one, 1,2,3,4-tetrahyd...	277	C18H15NO2	299962-12-2	32
5			1H-Indole-3-acetic acid, 5-[(tri...	277	C14H19NO3Si	072101-35-0	16

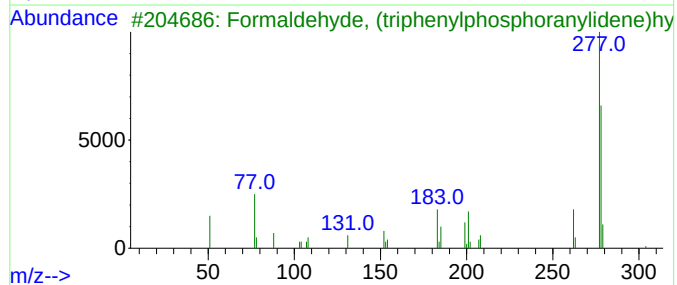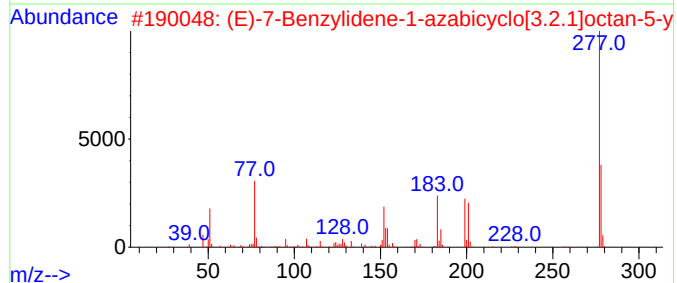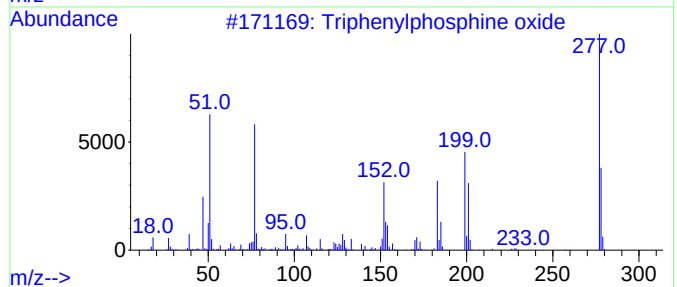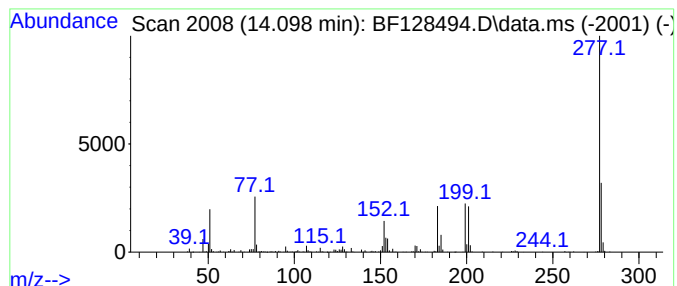

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052622\
Data File : BF128494.D
Acq On : 27 May 2022 01:52
Operator : CG\JU
Sample : PB145118BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145118BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.098	7.1	ng	683449	5	14.004	1916960	20.0