
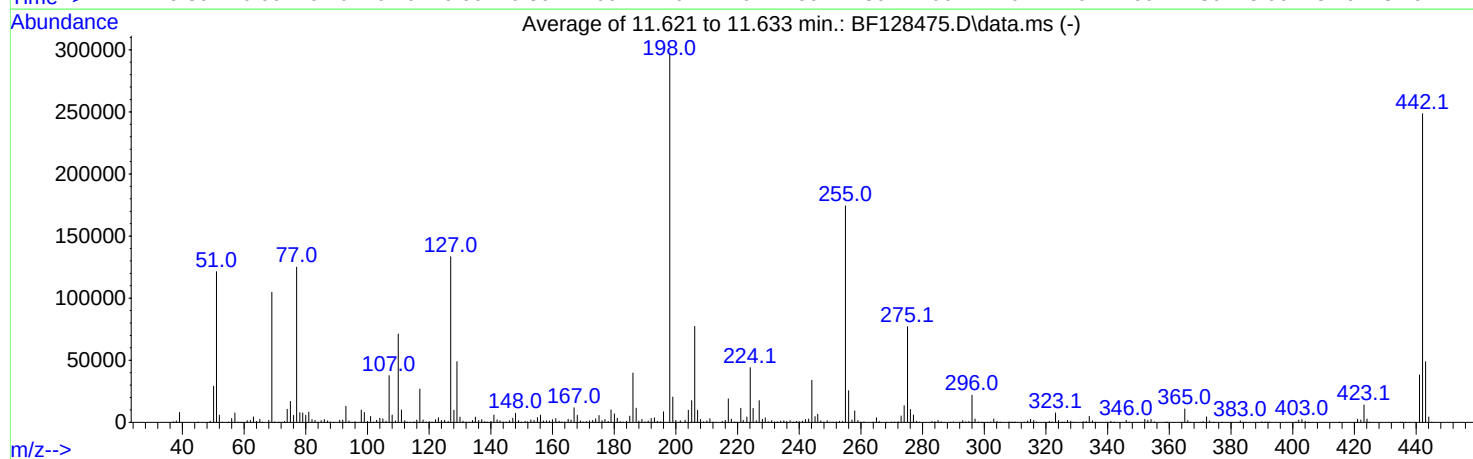


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052622\
 Data File : BF128475.D
 Acq On : 26 May 2022 16:00
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 27 01:51:59 2022

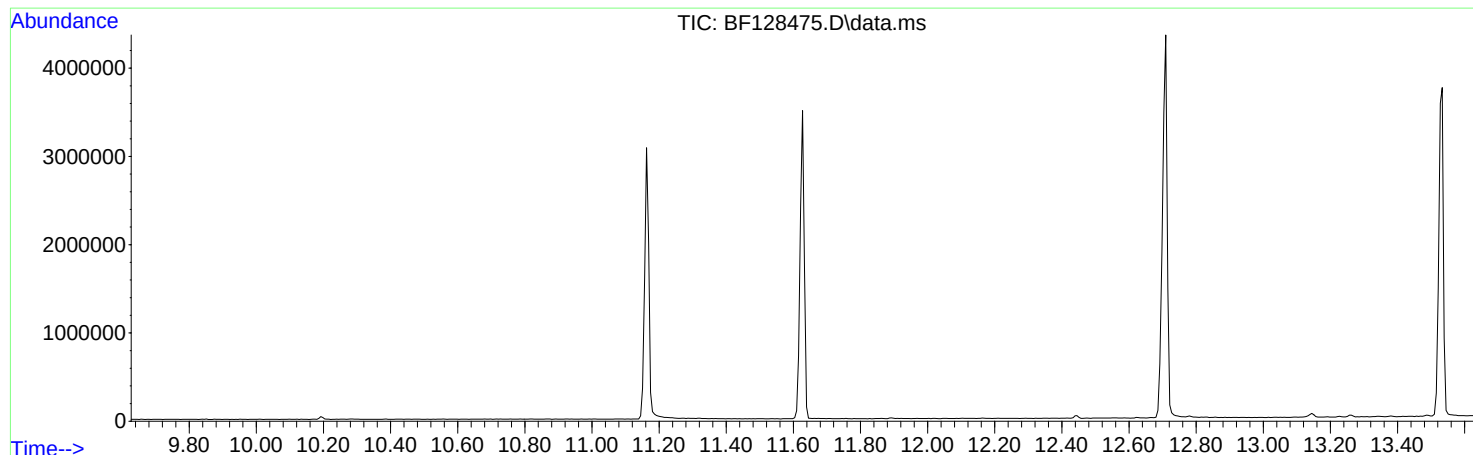




AutoFind: Scans 1587, 1588, 1589; Background Corrected with Scan 1581

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.0	121319	PASS
68	69	0.00	2	1.6	1700	PASS
69	198	0.00	100	35.4	104772	PASS
70	69	0.00	2	0.3	340	PASS
127	198	10	80	45.0	133379	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	296213	PASS
199	198	5	9	6.9	20401	PASS
275	198	10	60	26.0	77008	PASS
365	198	1	100	3.7	10879	PASS
441	198	0.01	100	12.9	38093	PASS
442	442	50	100	100.0	248555	PASS
443	442	15	24	19.6	48813	PASS

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052622\  
Data File : BF128475.D  
Acq On    : 26 May 2022  16:00  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 27 07:36:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Qlast Update : Fri May 27 01:51:59 2022
Response via : Initial Calibration

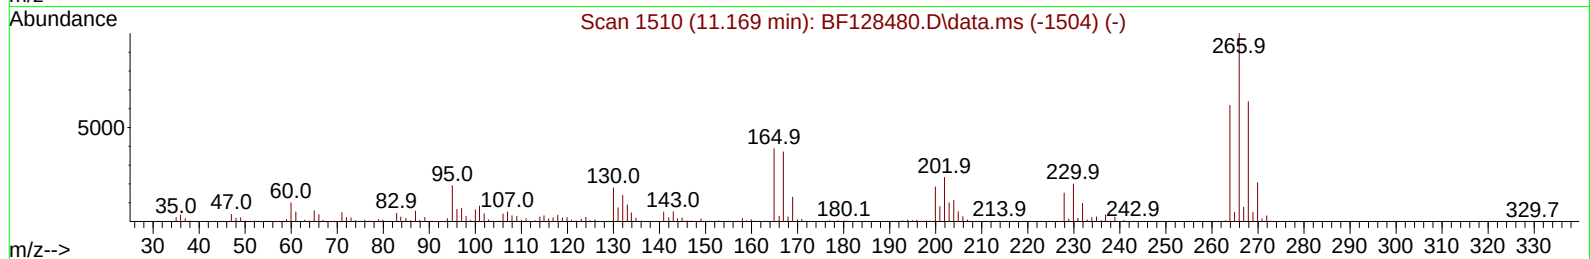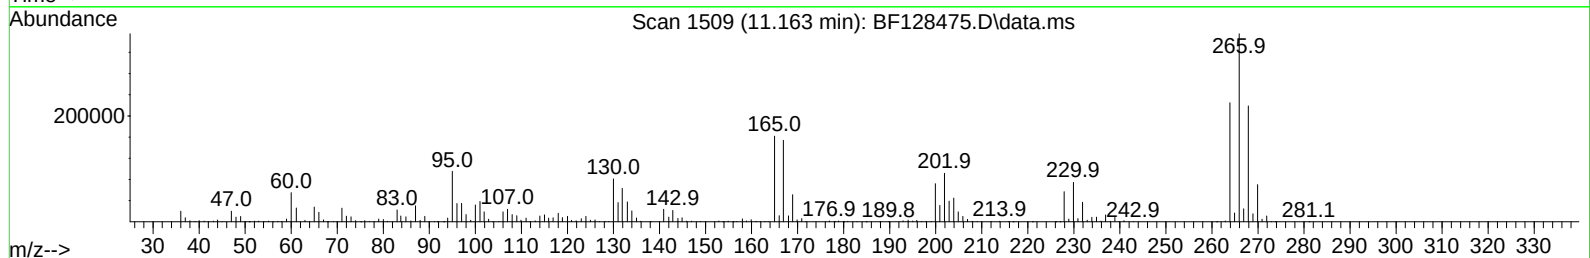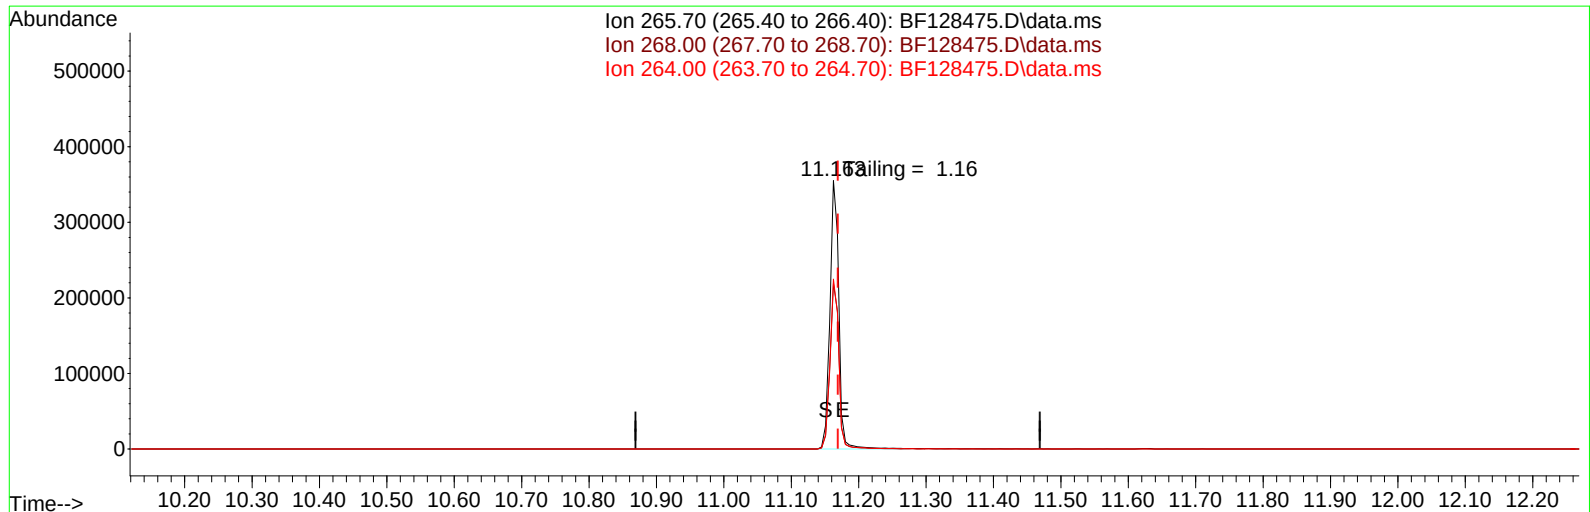

TIC: BF128475.D\data.ms

(70) Pentachlorophenol (C)

11.163min (-0.006) 386910.24 ng




response **325502**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	61.63
264.00	61.80	63.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052622\
 Data File : BF128475.D
 Acq On : 26 May 2022 16:00
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 27 07:36:20 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 27 01:51:59 2022
 Response via : Initial Calibration

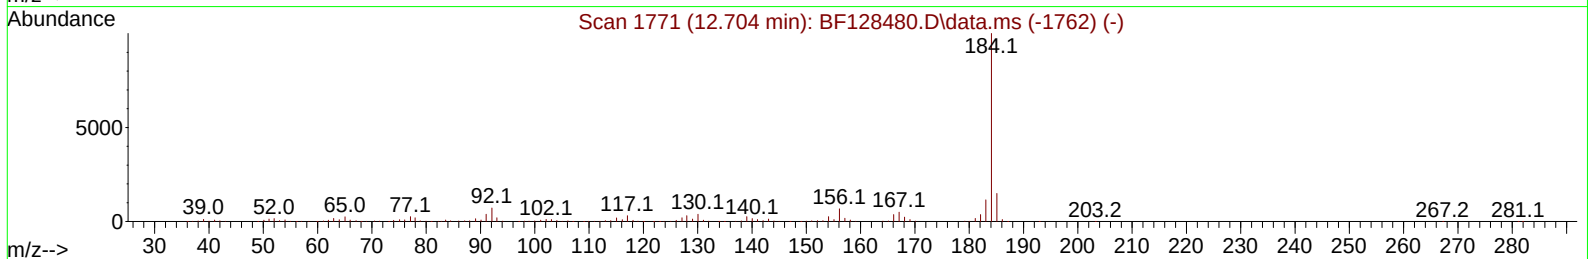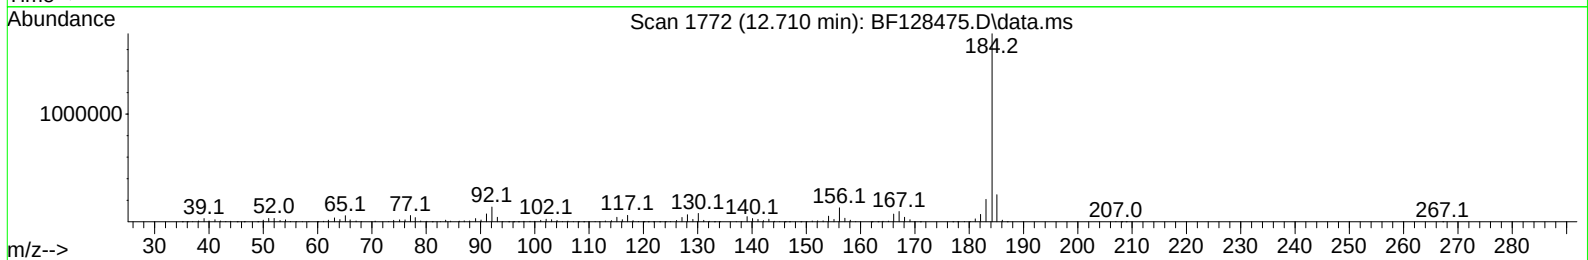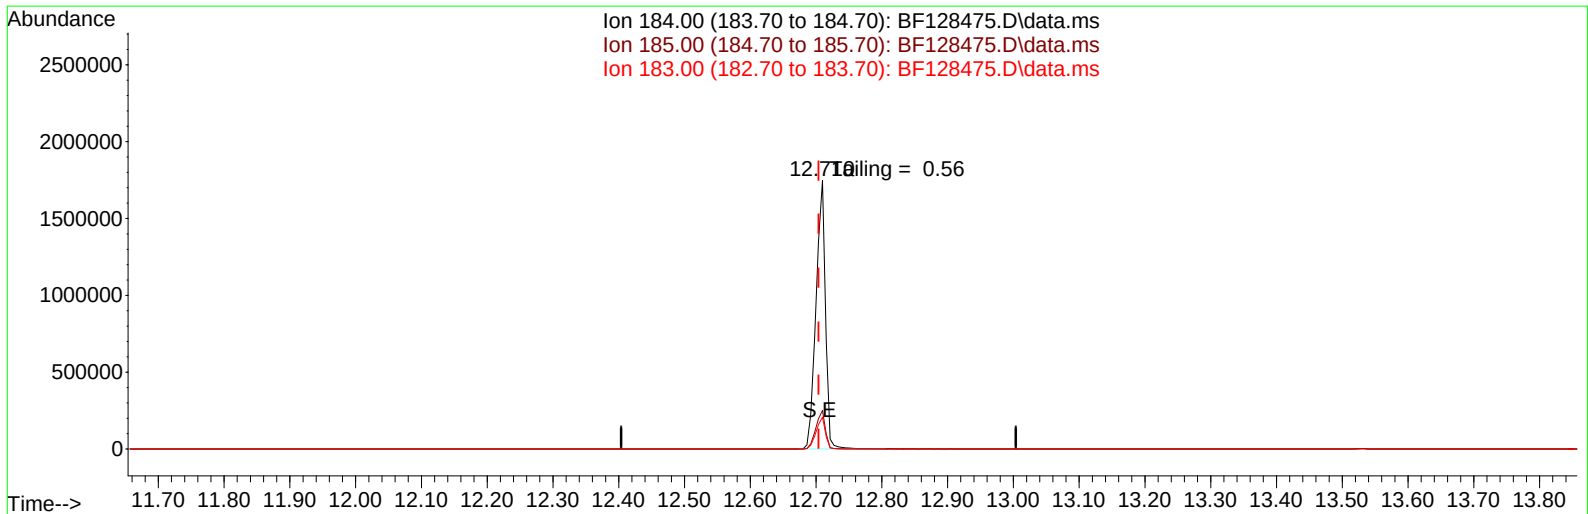

TIC: BF128475.D\data.ms

(77) Benzidine

12.710min (+ 0.006) 177280.10 ng

response 1741944

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.41
183.00	11.60	11.96
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/26/2022	BNA_F	<u>BF128475.D</u>
Compound Name	Response	Retention Time
DDT	633616	13.533
DDD	4252	13.262
DDE	0	12.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4252	637868	0.67

Instrument :
BNA_F
ClientSampleId :
DFTPP