
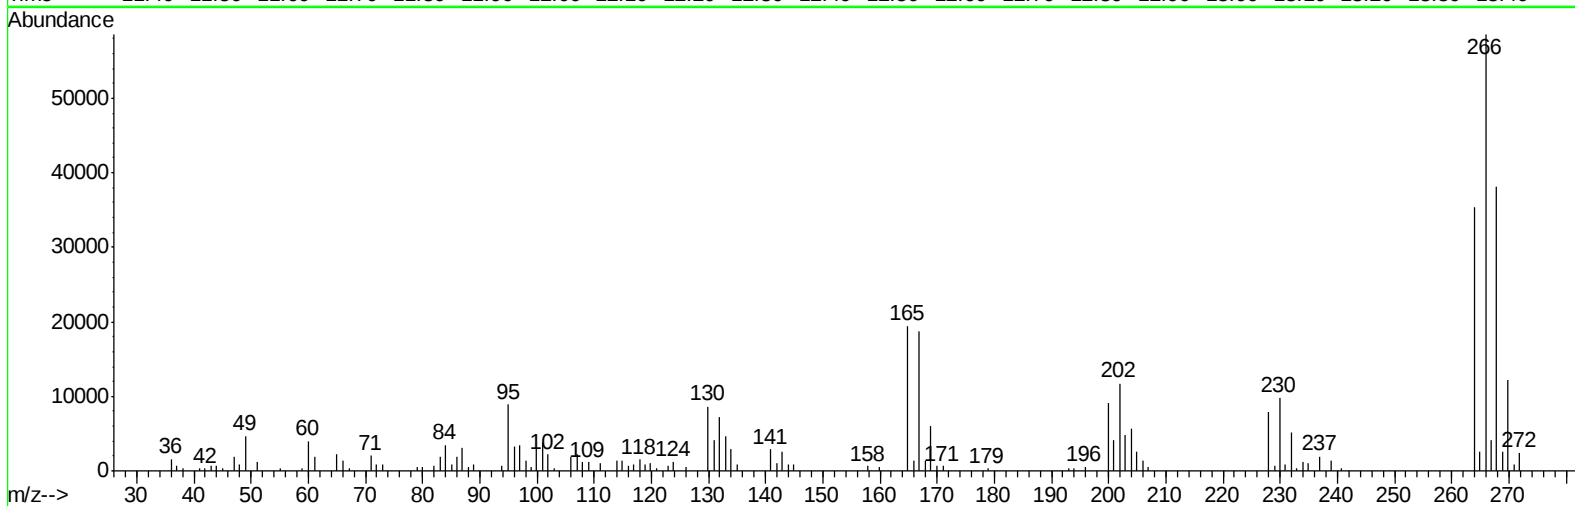


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052715\
Data File : BF079517.D
Acq On : 27 May 2015 13:54
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 28 05:25:49 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 28 00:48:25 2015
Response via : Initial Calibration

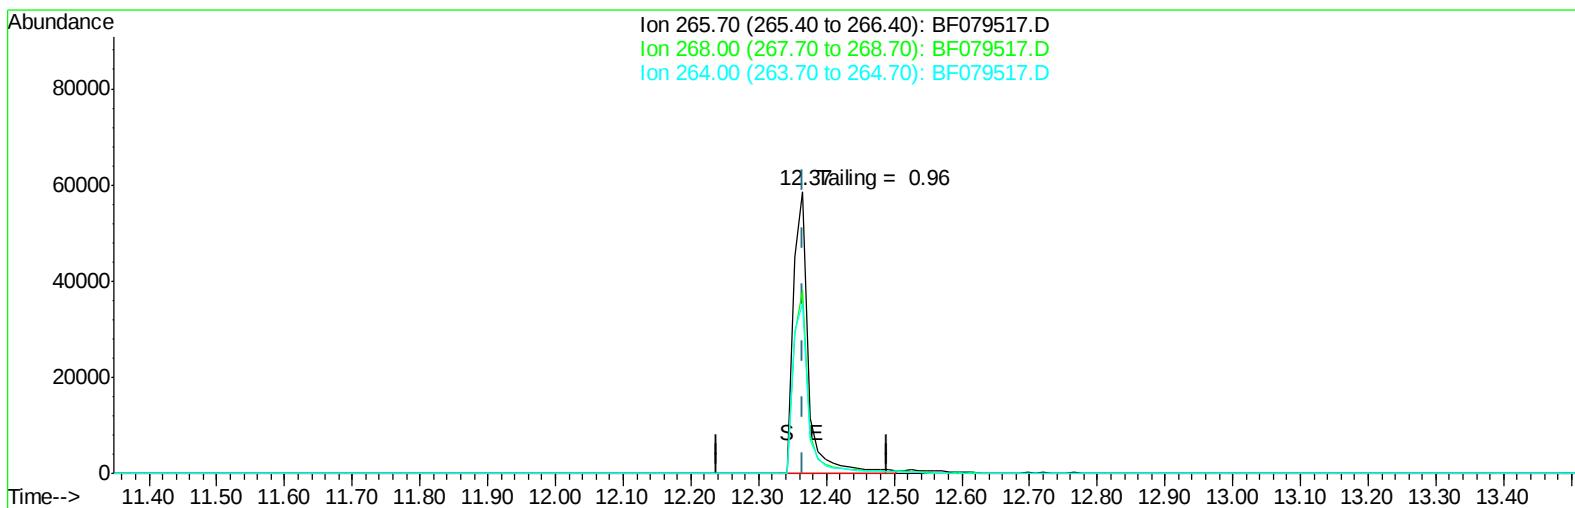

TIC: BF079517.D

(69) Pentachlorophenol (C)



12.365min (-0.000) 23379.20ng

response 91060

Ion	Exp%	Act%
265.70	100	100
268.00	70.10	65.06
264.00	62.50	60.37
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052715\
Data File : BF079517.D
Acq On : 27 May 2015 13:54
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 28 05:25:49 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 28 00:48:25 2015
Response via : Initial Calibration

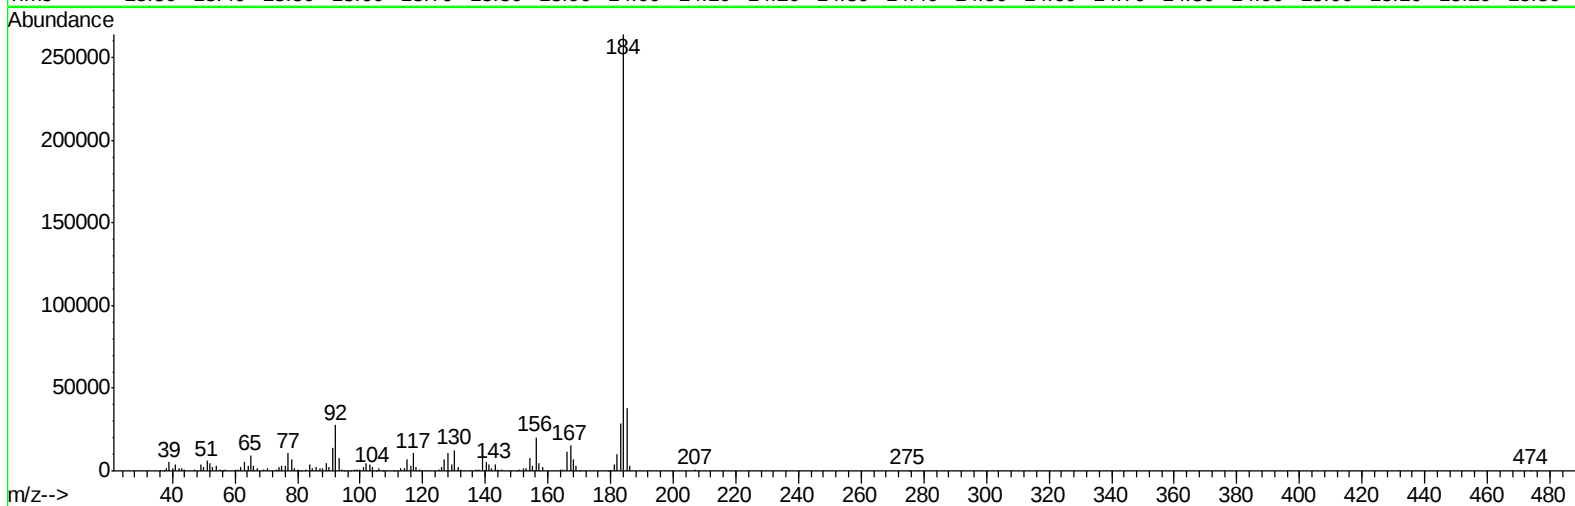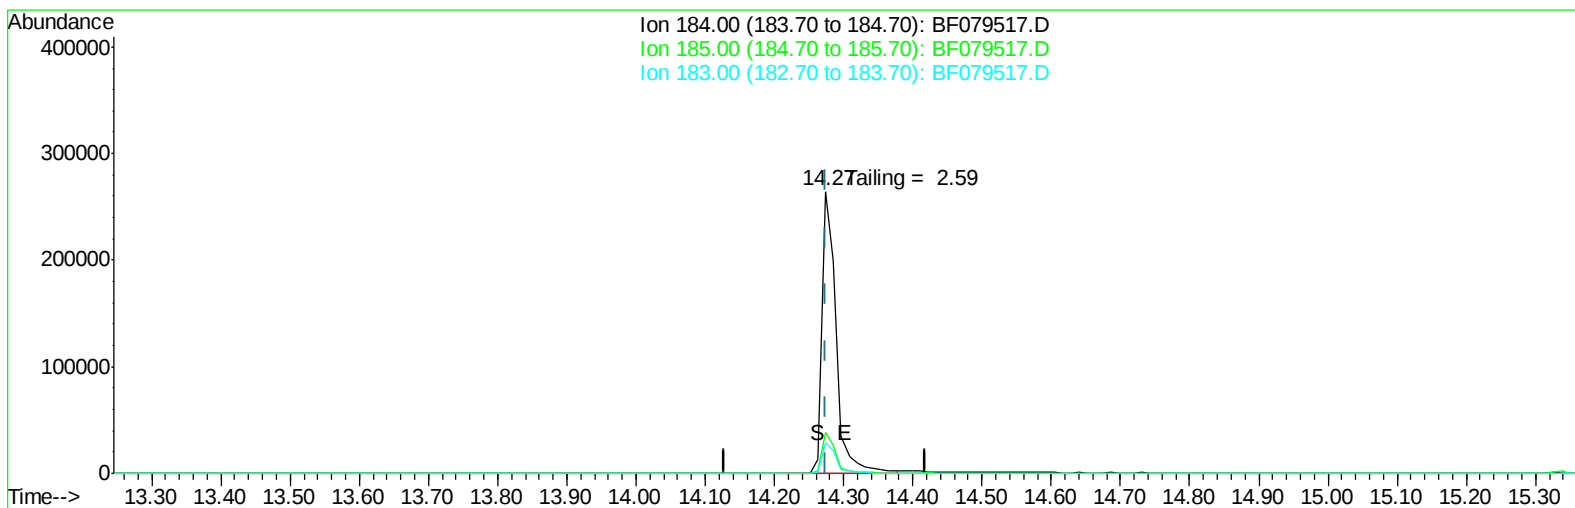

TIC: BF079517.D

(76) Benzidine

14.274min (-0.000) 74417.06ng

response 380948

Ion	Exp%	Act%
184.00	100	100
185.00	15.10	14.45
183.00	10.70	10.90
0.00	0.00	0.00