


Data Path : Z:\HPCHEM1\BNA_F\Data\BF052715\
 Data File : BF079517.D
 Acq On : 27 May 2015 13:54
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052615.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 28 00:48:25 2015

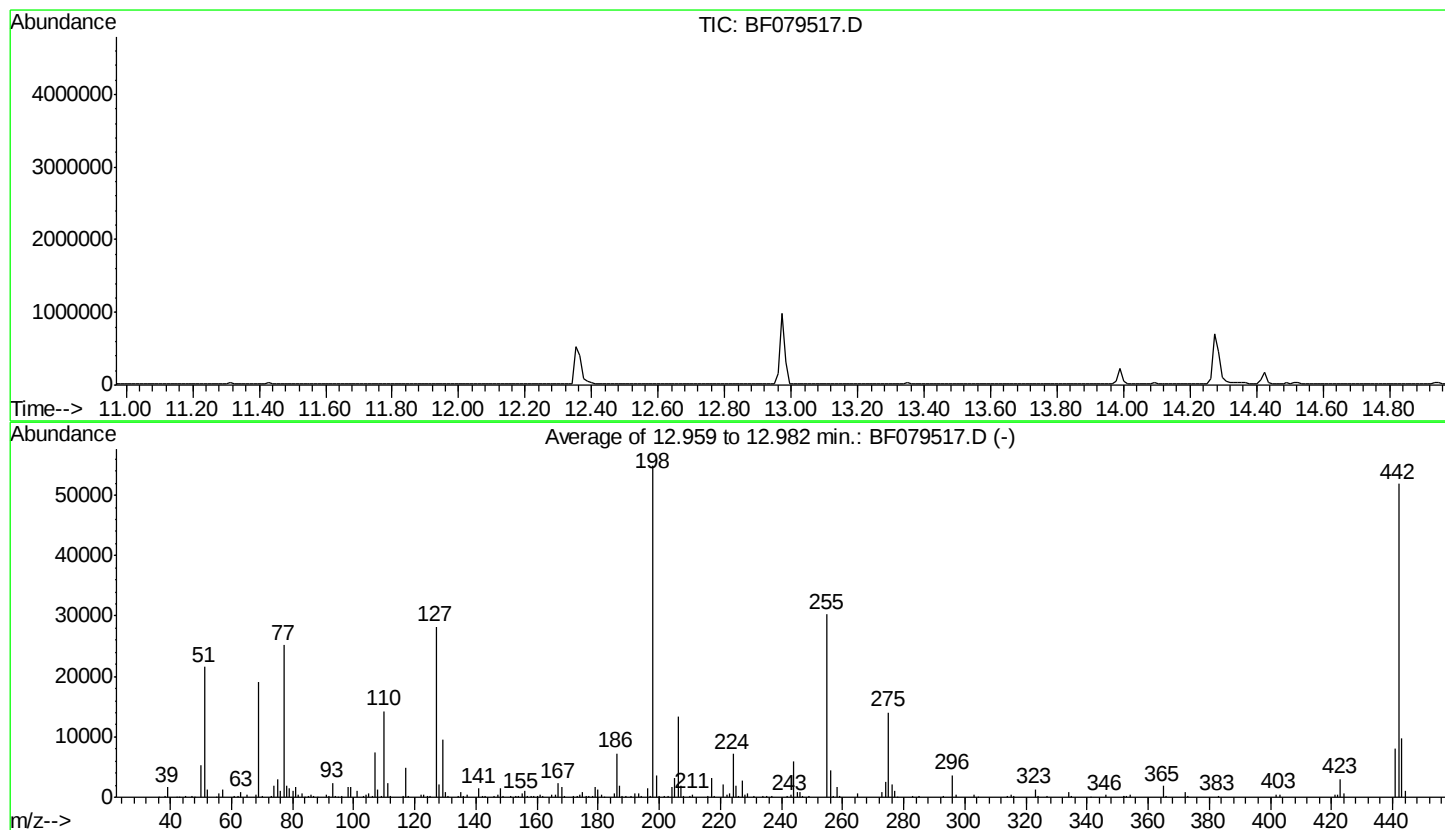

AutoFind: Scans 1030, 1031, 1032; Background Corrected with Scan 1027

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.3	21583	PASS
68	69	0.00	2	2.1	400	PASS
69	198	0.00	100	34.7	19055	PASS
70	69	0.00	2	0.7	133	PASS
127	198	10	80	51.4	28237	PASS
197	198	0.00	2	0.4	225	PASS
198	198	100	100	100.0	54893	PASS
199	198	5	9	6.6	3623	PASS
275	198	10	60	25.5	14005	PASS
365	198	1	100	3.4	1847	PASS
441	442	0.01	24	15.6	8098	PASS
442	198	50	100	94.5	51892	PASS
443	442	15	24	18.9	9832	PASS