
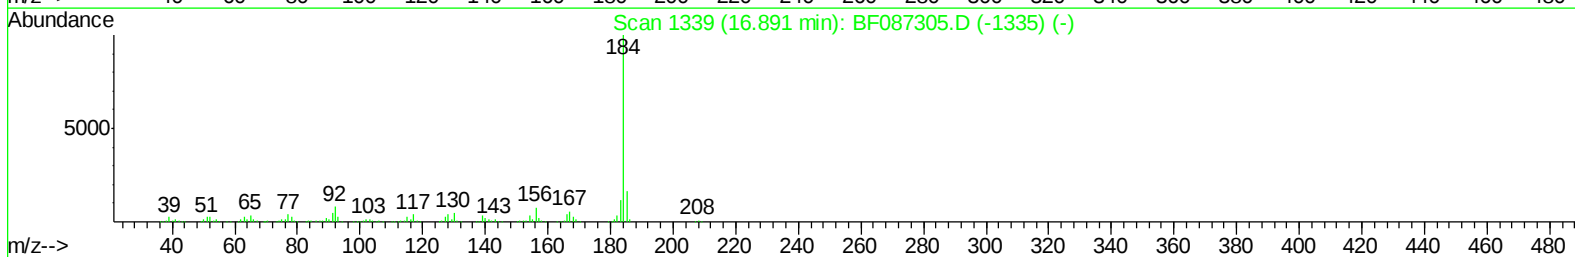
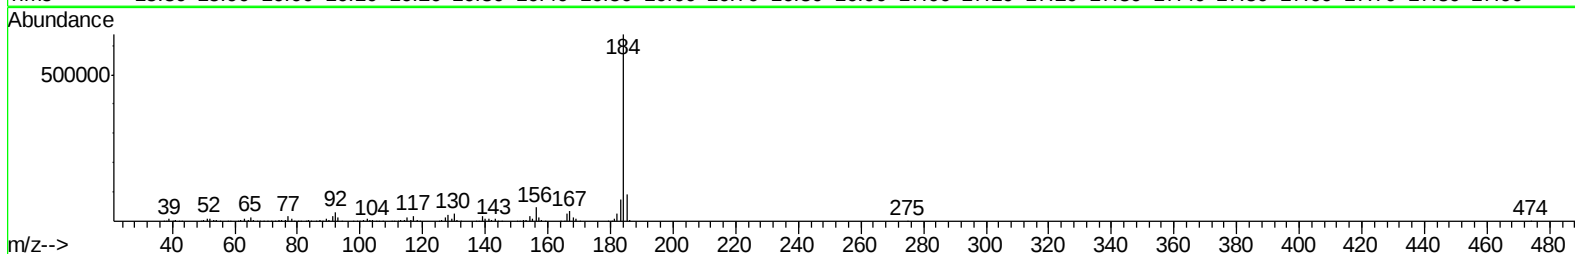


Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF052716\  
Data File : BF087463.D  
Acq On : 28 May 2016 2:38  
Operator : UM/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 30 01:25:01 2016  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF052316.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon May 30 00:59:34 2016  
Response via : Initial Calibration

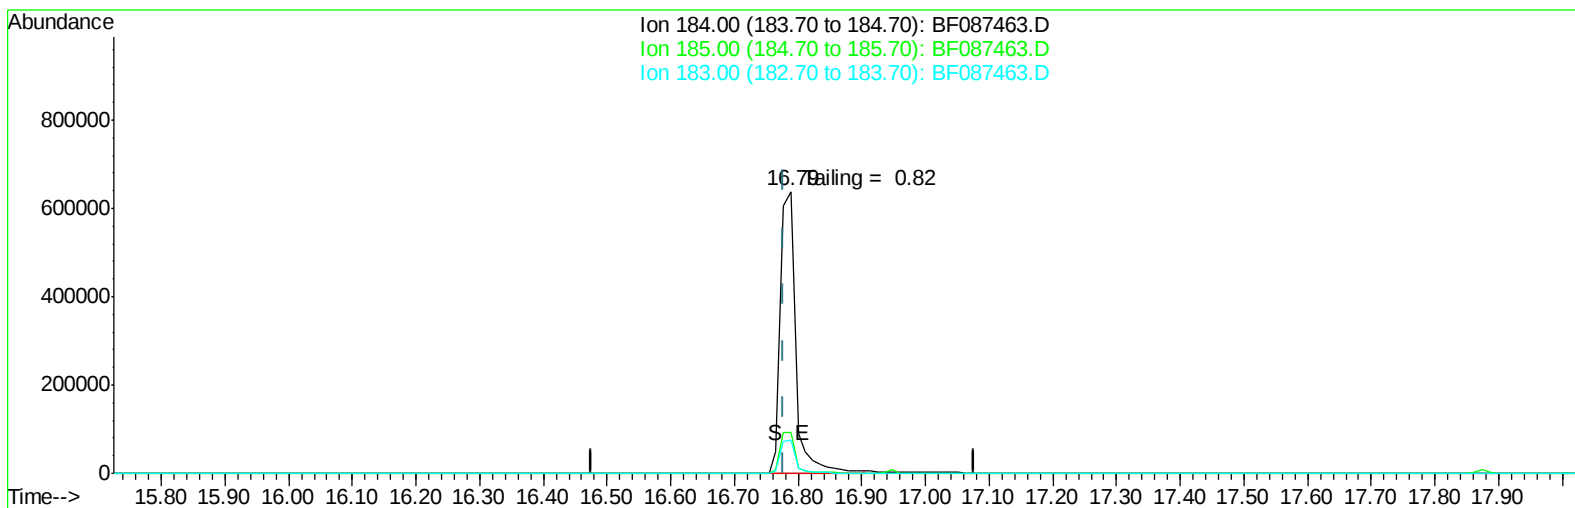

TIC: BF087463.D

(76) Benzidine




16.788min (+0.012) 0.00ng

response 1075165

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 17.00 | 14.34 |
| 183.00 | 12.20 | 11.89 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF052716\  
Data File : BF087463.D  
Acq On : 28 May 2016 2:38  
Operator : UM/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 30 01:25:01 2016  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF052316.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon May 30 00:59:34 2016  
Response via : Initial Calibration

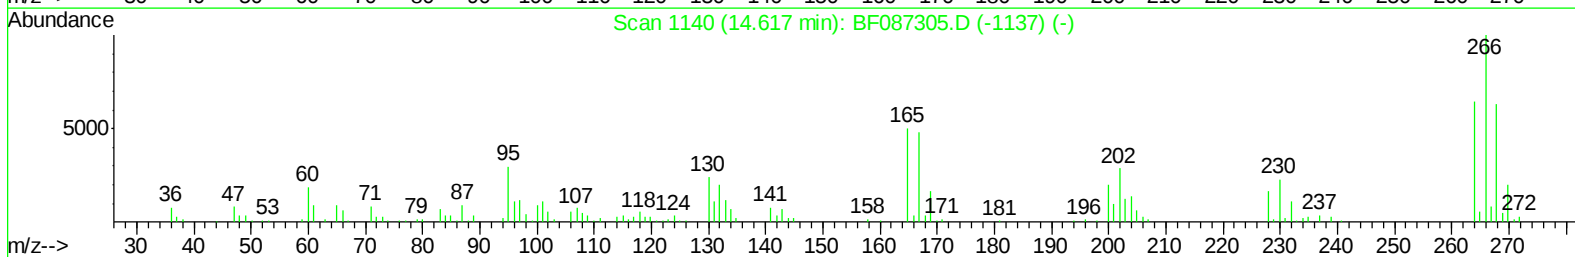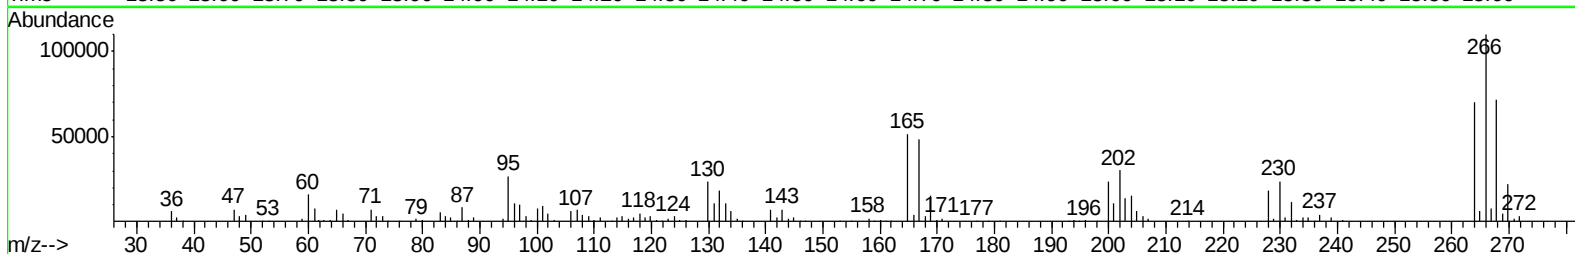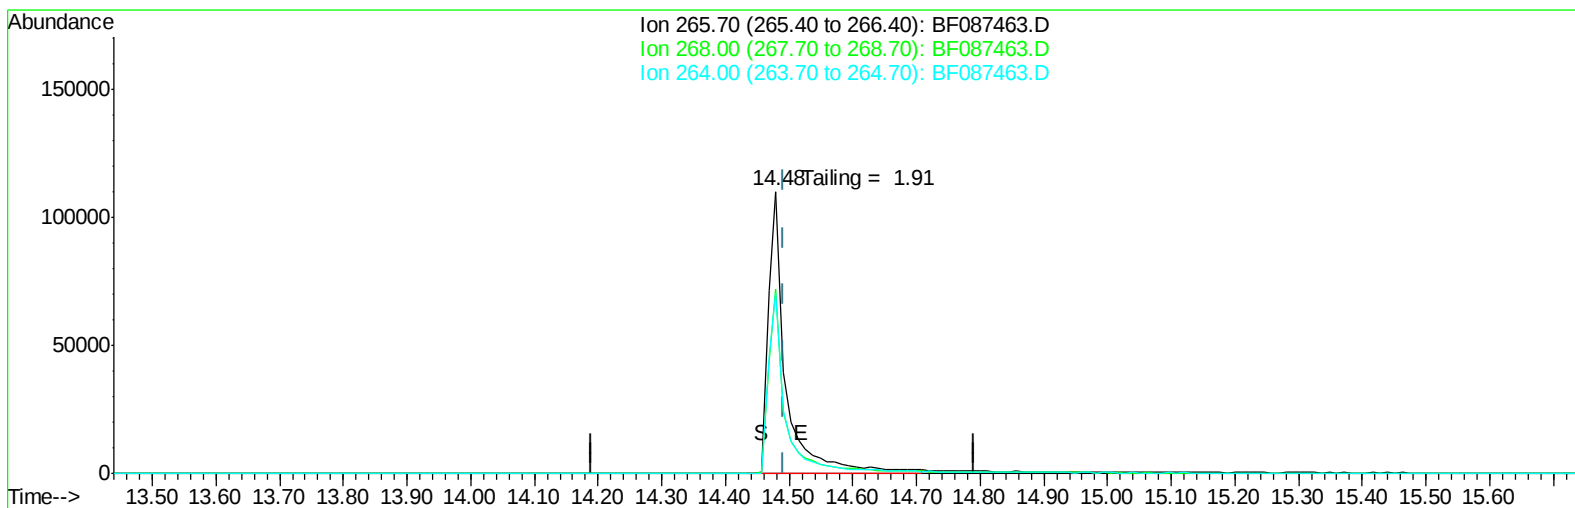

TIC: BF087463.D

(69) Pentachlorophenol (C)

14.480min (-0.011) 0.00ng

response 215749

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 64.40 | 65.29 |
| 264.00 | 66.10 | 63.95 |
| 0.00   | 0.00  | 0.00  |