


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052716\
 Data File : BF087463.D
 Acq On : 28 May 2016 2:38
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 25 16:26:52 2016

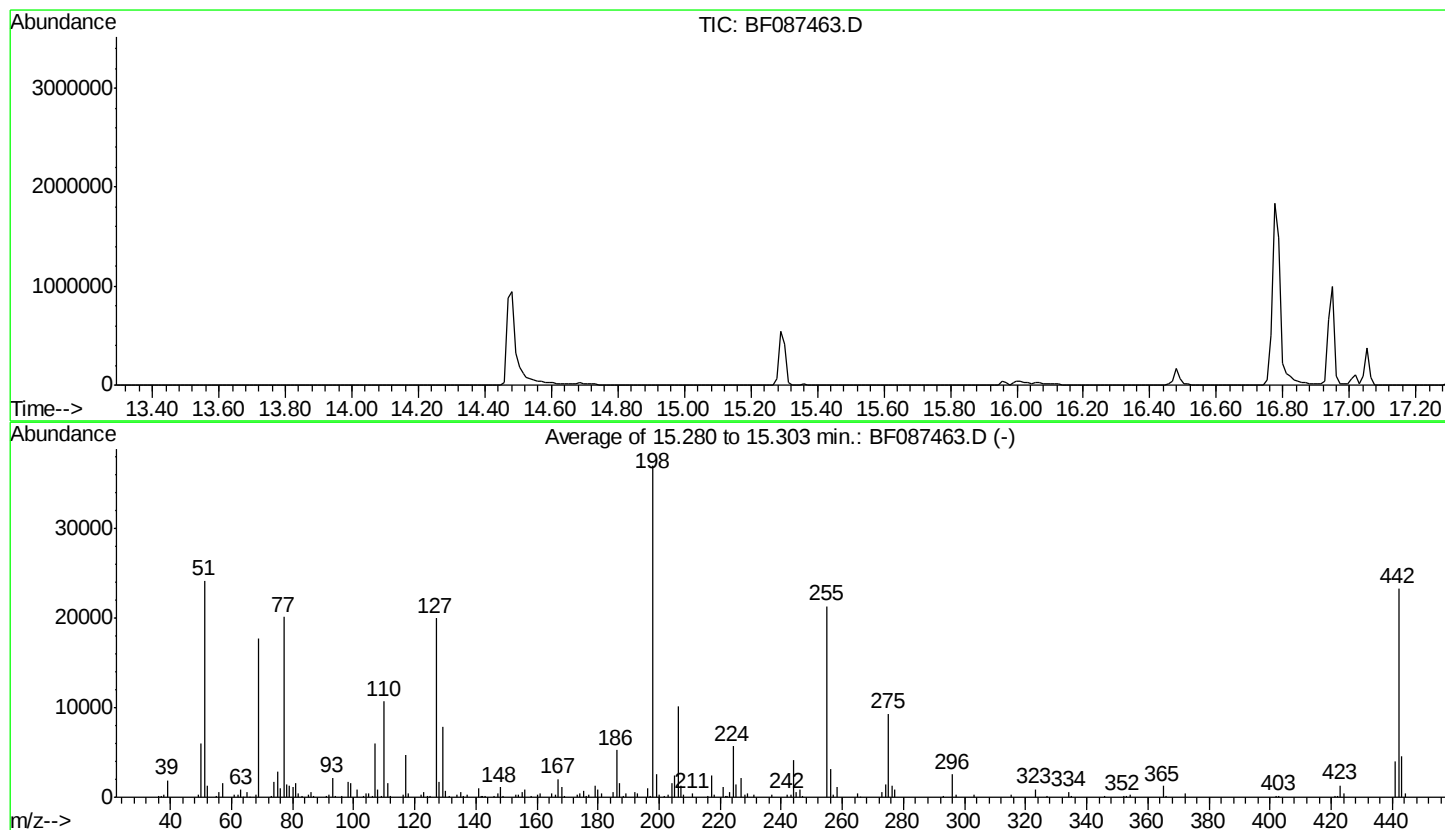

AutoFind: Scans 1198, 1199, 1200; Background Corrected with Scan 1195

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	65.4	24151	PASS
68	69	0.00	2	1.4	244	PASS
69	198	0.00	100	48.0	17750	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.9	19921	PASS
197	198	0.00	2	0.3	118	PASS
198	198	100	100	100.0	36949	PASS
199	198	5	9	6.9	2544	PASS
275	198	10	60	25.2	9302	PASS
365	198	1	100	3.3	1227	PASS
441	442	0.01	24	17.3	4019	PASS
442	198	50	100	62.9	23227	PASS
443	442	15	24	19.4	4502	PASS