


Data Path : Z:\HPCHEM1\BNA F\Data\BF052717\
Data File : BF095498.D
Acq On : 27 May 2017 13:01
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 30 00:43:33 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 26 16:50:16 2017
Response via : Initial Calibration

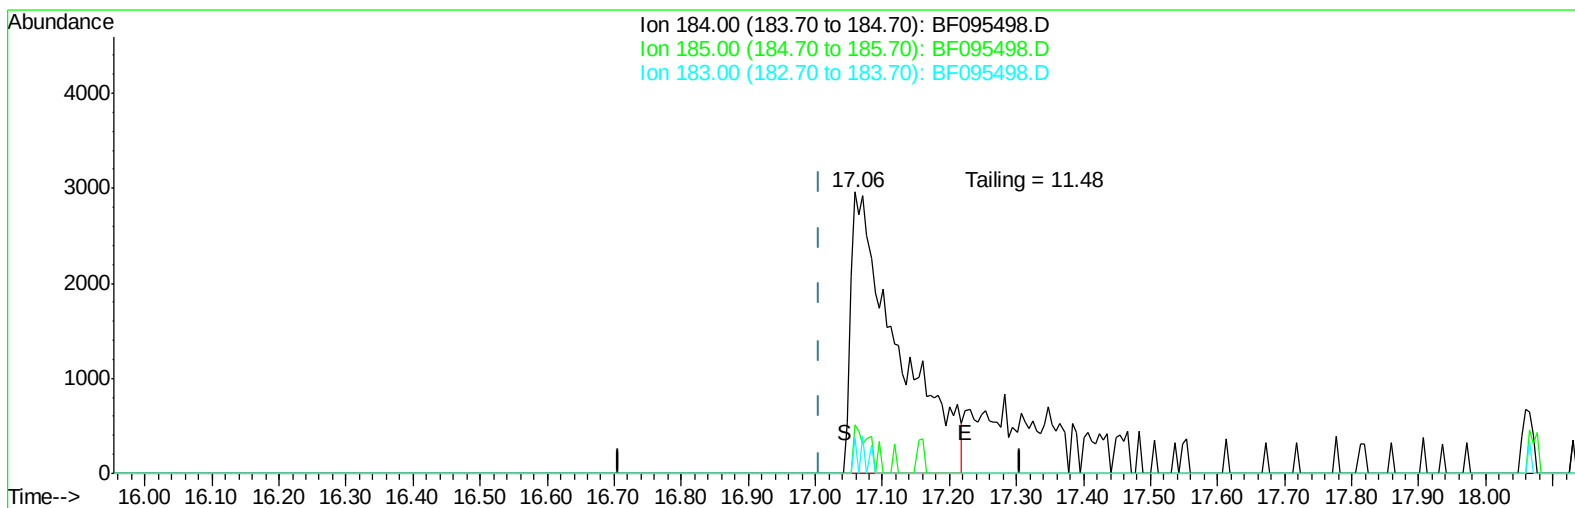

TIC: BF095498.D

(76) Benzidine



17.059min (+0.053) 2254.96ng

response 10361

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	17.18
183.00	12.20	12.55
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF052717\
Data File : BF095498.D
Acq On : 27 May 2017 13:01
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 30 00:43:33 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 26 16:50:16 2017
Response via : Initial Calibration

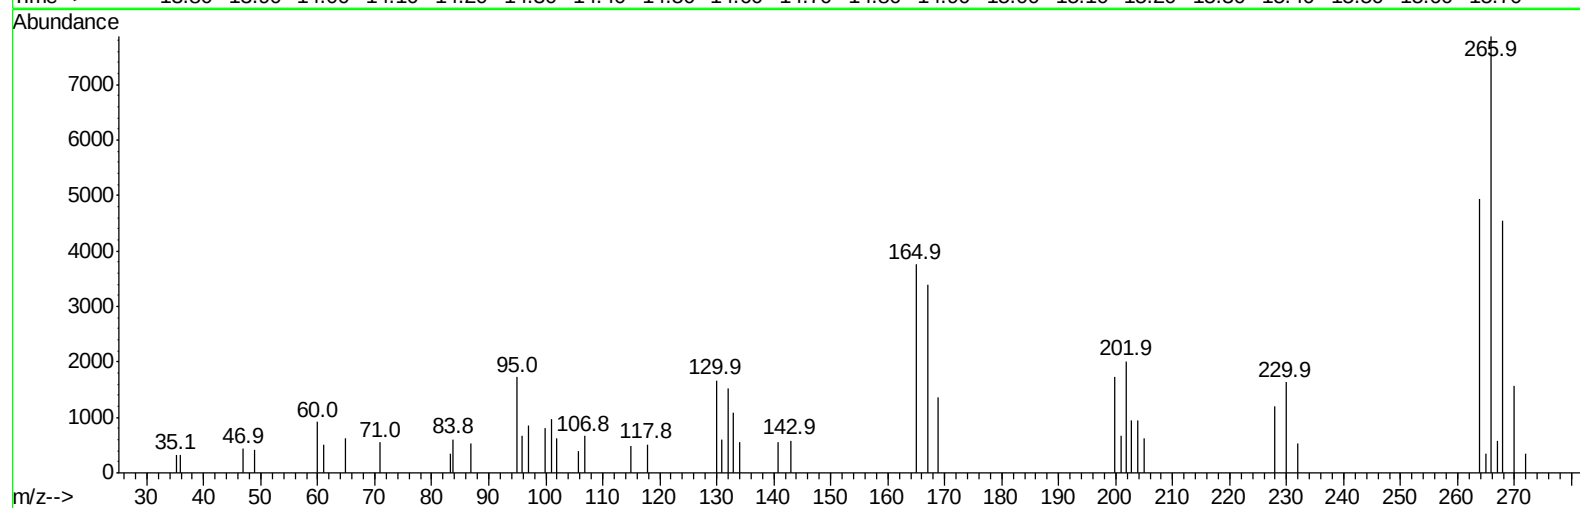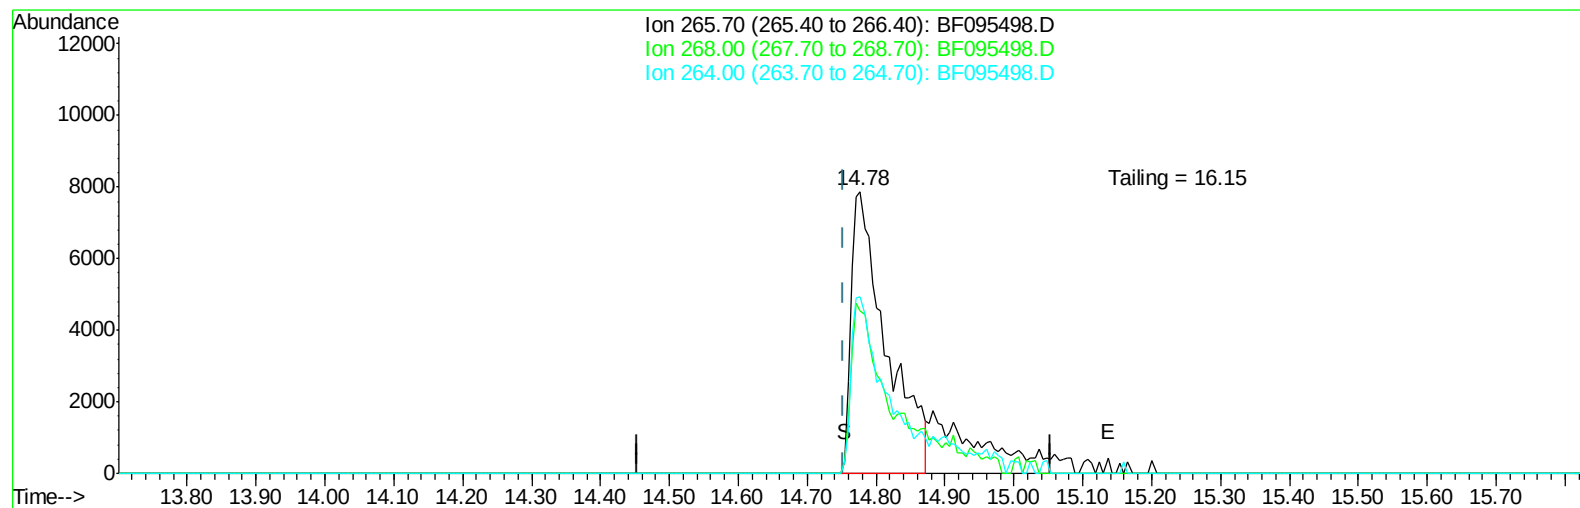

TIC: BF095498.D

(69) Pentachlorophenol (C)

14.777min (+0.024) 0.00ng m

response 27704

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	57.70
264.00	64.60	62.77
0.00	0.00	0.00